

## PATENT COOPERATION TREATY

PCT

From the INTERNATIONAL BUREAU

NOTIFICATION OF THE RECORDING  
OF A CHANGE(PCT Rule 92bis.1 and  
Administrative Instructions, Section 422)

To:

HEDBERG, Åke  
Aros Patent AB  
P.O. Box 1544  
S-751 45 Uppsala  
SUÈDEDate of mailing (day/month/year)  
03 August 2001 (03.08.01)Applicant's or agent's file reference  
P170PC00

## IMPORTANT NOTIFICATION

International application No.  
PCT/SE00/01109International filing date (day/month/year)  
30 May 2000 (30.05.00)

## 1. The following indications appeared on record concerning:

☒ the applicant ☐ the inventor ☐ the agent ☐ the common representative

Name and Address

SCANDITRONIX MEDICAL AB  
Stålgatan 14  
S-754 50 Uppsala  
Sweden

State of Nationality

SE

State of Residence

SE

Telephone No.

Facsimile No.

Teleprinter No.

## 2. The International Bureau hereby notifies the applicant that the following change has been recorded concerning:

☐ the person ☐ the name ☐ the address ☐ the nationality ☐ the residence

Name and Address

State of Nationality

State of Residence

Telephone No.

Facsimile No.

Teleprinter No.

## 3. Further observations, if necessary:

**Applicant box 1 deleted from record. NÄFSTADIUS Peter now recorded as applicant/inventor  
for all designated states.**

## 4. A copy of this notification has been sent to:

☒ the receiving Office ☐ the designated Offices concerned  
☐ the International Searching Authority ☒ the elected Offices concerned  
☒ the International Preliminary Examining Authority ☐ other:The International Bureau of WIPO  
34, chemin des Colombettes  
1211 Geneva 20, Switzerland

Authorized officer

Marie-Thérèse Priser

## PATENT COOPERATION TREATY

PCT

## NOTIFICATION OF ELECTION

(PCT Rule 61.2)

From the INTERNATIONAL BUREAU

To:

Commissioner  
 US Department of Commerce  
 United States Patent and Trademark  
 Office, PCT  
 2011 South Clark Place Room  
 CP2/5C24  
 Arlington, VA 22202  
 ETATS-UNIS D'AMERIQUE  
 in its capacity as elected Office

Date of mailing (day/month/year)  
 07 February 2001 (07.02.01)

International application No.  
 PCT/SE00/01109

Applicant's or agent's file reference  
 P170PC00

International filing date (day/month/year)  
 30 May 2000 (30.05.00)

Priority date (day/month/year)  
 09 June 1999 (09.06.99)

Applicant

NÄFSTADIUS, Peder

1. The designated Office is hereby notified of its election made:

☒ in the demand filed with the International Preliminary Examining Authority on:  
 06 December 2000 (06.12.00)

☐ in a notice effecting later election filed with the International Bureau on:

2. The election ☒ was

☐ was not

made before the expiration of 19 months from the priority date or, where Rule 32 applies, within the time limit under Rule 32.2(b).

The International Bureau of WIPO  
 34, chemin des Colombettes  
 1211 Geneva 20, Switzerland

Facsimile No. (41-22) 740 14 35

Authorized officer

Catherine Massetti

Telephone No. (41-22) 338 83 38

## PATENT COOPERATION TREATY

PCT

## INTERNATIONAL PRELIMINARY EXAMINATION REPORT

(PCT Article 36 and Rule 70)



Applicant's or agent's file reference <b>P170PC</b>	<b>FOR FURTHER ACTION</b> See Notification of Transmittal of International Preliminary Examination Report (Form PCT/IPEA/416)	
International application No. <b>PCT/SE00/01109</b>	International filing date (day/month/year) <b>30.05.2000</b>	Priority date (day/month/year) <b>09.06.1999</b>
International Patent Classification (IPC) or national classification and IPC <b>A 61 N 5/01, A 61 B 6/04</b>		
Applicant <b>Scanditronix Medical AB et al] Nätstadius, Peder</b>		

1. This international preliminary examination report has been prepared by this International Preliminary Examining Authority and is transmitted to the applicant according to Article 36.

2. This REPORT consists of a total of 3 sheets, including this cover sheet.

☐ This report is also accompanied by ANNEXES, i.e., sheets of the description, claims and/or drawings which have been amended and are the basis for this report and/or sheets containing rectifications made before this Authority (see Rule 70.16 and Section 607 of the Administrative Instructions under the PCT).

These annexes consist of a total of \_\_\_\_\_ sheets.

3. This report contains indications relating to the following items:

- I ☒ Basis of the report
- II ☐ Priority
- III ☐ Non-establishment of opinion with regard to novelty, inventive step and industrial applicability
- IV ☐ Lack of unity of invention
- V ☒ Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement
- VI ☐ Certain documents cited
- VII ☐ Certain defects in the international application
- VIII ☐ Certain observations on the international application

Date of submission of the demand <b>06.12.2000</b>	Date of completion of this report <b>18.10.2001</b>
Name and mailing address of the IPEA/SE Patent- och registreringsverket Box 5055 S-102 42 STOCKHOLM Facsimile No. 08-667 72 88	Authorized officer <b>Monika Bohlin/Els</b> Telephone No. 08-782 25 00

# INTERNATIONAL PRELIMINARY EXAMINATION REPORT

International application No.

PCT/SE00/01109

## I. Basis of the report

### 1. With regard to the elements of the international application:\*

- ☒ the international application as originally filed
- ☐ the description:  
 pages \_\_\_\_\_, as originally filed  
 pages \_\_\_\_\_, filed with the demand  
 pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the claims:  
 pages \_\_\_\_\_, as originally filed  
 pages \_\_\_\_\_, as amended (together with any statement) under article 19  
 pages \_\_\_\_\_, filed with the demand  
 pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the drawings:  
 pages \_\_\_\_\_, as originally filed  
 pages \_\_\_\_\_, filed with the demand  
 pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the sequence listing part of the description:  
 pages \_\_\_\_\_, as originally filed  
 pages \_\_\_\_\_, filed with the demand  
 pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_

### 2. With regard to the language, all the elements marked above were available or furnished to this Authority in the language in which the international application was filed, unless otherwise indicated under this item. These elements were available or furnished to this Authority in the following language \_\_\_\_\_ which is:

- ☐ the language of a translation furnished for the purposes of international search (under Rule 23.1(b)).
- ☐ the language of publication of the international application (under Rule 48.3(b)).
- ☐ the language of the translation furnished for the purposes of international preliminary examination (under Rules 55.2 and/or 55.3).

### 3. With regard to any nucleotide and/or amino acid sequence disclosed in the international application, the international preliminary examination was carried out on the basis of the sequence listing:

- ☐ contained in the international application in written form.
- ☐ filed together with the international application in computer readable form.
- ☐ furnished subsequently to this Authority in written form.
- ☐ furnished subsequently to this Authority in computer readable form.
- ☐ The statement that the subsequently furnished written sequence listing does not go beyond the disclosure in the international application as filed has been furnished.
- ☐ The statement that the information recorded in computer readable form is identical to the written sequence listing has been furnished.

### 4. ☐ The amendments have resulted in the cancellation of:

- ☐ the description, pages \_\_\_\_\_
- ☐ the claims, Nos. \_\_\_\_\_
- ☐ the drawings, sheet/fig \_\_\_\_\_

### 5. ☐ This report has been established as if (some of) the amendments had not been made, since they have been considered to go beyond the disclosure as filed, as indicated in the Supplemental Box (Rule 70.2 (c)).\*\*

\* Replacement sheets which have been furnished to the receiving Office in response to an invitation under Article 14 are referred to in this report as "originally filed" and are annexed to this report since they do not contain amendments (Rules 70.16 and 70.17).

\*\* Any replacement sheet containing such amendments must be referred to under item 1 and annexed to this report.

# INTERNATIONAL PRELIMINARY EXAMINATION REPORT

International application No.

PCT/SE00/01109

## V. Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement

### 1. Statement

Novelty (N)	Claims	<u>1-20</u>	YES
	Claims		NO
Inventive step (IS)	Claims	<u>1-20</u>	YES
	Claims		NO
Industrial applicability (IA)	Claims	<u>1-20</u>	YES
	Claims		NO

### 2. Citations and explanations (Rule 70.7)

#### Cited documents:

D1 US 4741015 A,  
D2 WO 8908269 A1  
D3 US 5751781 A  
D4 FR 2529088 A1  
D5 GB 1129653 A

The documents cited in the International Search Report represent background art.

The invention defined in claims 1-20 is not disclosed in any of these documents.

None of the cited documents gives any indication towards the claimed radiation gantry. No relevant combination of the cited documents would lead a person skilled in the art to the invention defined in the claims.

Therefore, the invention defined in claims 1-20 is novel and is considered to involve an inventive step. It is also considered to be industrially applicable.

## PATENT COOPERATION TREATY

PCT

NOTIFICATION CONCERNING  
SUBMISSION OR TRANSMITTAL  
OF PRIORITY DOCUMENT

(PCT Administrative Instructions, Section 411)

From the INTERNATIONAL BUREAU

To:

HEDBERG, Åke  
Aros Patent AB  
P.O. Box 1544  
S-751 45 Uppsala  
SUÈDE

Date of mailing (day/month/year) 12 October 2001 (12.10.01)	<b>IMPORTANT NOTIFICATION</b>
Applicant's or agent's file reference P170PC00	
International application No. PCT/SE00/01109	International filing date (day/month/year) 30 May 2000 (30.05.00)
International publication date (day/month/year) 14 December 2000 (14.12.00)	Priority date (day/month/year) 09 June 1999 (09.06.99)
Applicant NÄFSTADIUS, Peder	

1. The applicant is hereby notified of the date of receipt (except where the letters "NR" appear in the right-hand column) by the International Bureau of the priority document(s) relating to the earlier application(s) indicated below. Unless otherwise indicated by an asterisk appearing next to a date of receipt, or by the letters "NR", in the right-hand column, the priority document concerned was submitted or transmitted to the International Bureau in compliance with Rule 17.1(a) or (b).
2. This updates and replaces any previously issued notification concerning submission or transmittal of priority documents.
3. An asterisk(\*) appearing next to a date of receipt, in the right-hand column, denotes a priority document submitted or transmitted to the International Bureau but not in compliance with Rule 17.1(a) or (b). In such a case, **the attention of the applicant is directed** to Rule 17.1(c) which provides that no designated Office may disregard the priority claim concerned before giving the applicant an opportunity, upon entry into the national phase, to furnish the priority document within a time limit which is reasonable under the circumstances.
4. The letters "NR" appearing in the right-hand column denote a priority document which was not received by the International Bureau or which the applicant did not request the receiving Office to prepare and transmit to the International Bureau, as provided by Rule 17.1(a) or (b), respectively. In such a case, **the attention of the applicant is directed** to Rule 17.1(c) which provides that no designated Office may disregard the priority claim concerned before giving the applicant an opportunity, upon entry into the national phase, to furnish the priority document within a time limit which is reasonable under the circumstances.

<u>Priority date</u>	<u>Priority application No.</u>	<u>Country or regional Office or PCT receiving Office</u>	<u>Date of receipt of priority document</u>
09 June 1999 (09.06.99)	9902163-6	SE	04 Augu 2000 (04.08.00)

The International Bureau of WIPO  
34, chemin des Colombettes  
1211 Geneva 20, Switzerland

Facsimile No. (41-22) 740.14.35

Authorized officer

N. Masson

Telephone No. (41-22) 338.83.38

# PATENT COOPERATION TREATY

## PCT

### INTERNATIONAL PRELIMINARY EXAMINATION REPORT

(PCT Article 36 and Rule 70)

Applicant's or agent's file reference <b>P170PC</b>	<b>FOR FURTHER ACTION</b> See Notification of Transmittal of International Preliminary Examination Report (Form PCT/IPEA/416)	
International application No. <b>PCT/SE00/01109</b>	International filing date (day/month/year) <b>30.05.2000</b>	Priority date (day/month/year) <b>09.06.1999</b>
International Patent Classification (IPC) or national classification and IPC <sub>7</sub> <b>A 61 N 5/01, A 61 B 6/04</b>		
Applicant <b>Scanditronix Medical AB et al</b>		

<ol style="list-style-type: none"> <li>1. This international preliminary examination report has been prepared by this International Preliminary Examining Authority and is transmitted to the applicant according to Article 36.</li> <li>2. This REPORT consists of a total of <u>  3  </u> sheets, including this cover sheet.   <input type="checkbox"/> This report is also accompanied by ANNEXES, i.e., sheets of the description, claims and/or drawings which have been amended and are the basis for this report and/or sheets containing rectifications made before this Authority (see Rule 70.16 and Section 607 of the Administrative Instructions under the PCT).             These annexes consist of a total of <u>          </u> sheets.         </li> <li>3. This report contains indications relating to the following items:             <table style="margin-left: 20px; border: none;"> <tr><td>I</td><td><input checked="" type="checkbox"/></td><td>Basis of the report</td></tr> <tr><td>II</td><td><input type="checkbox"/></td><td>Priority</td></tr> <tr><td>III</td><td><input type="checkbox"/></td><td>Non-establishment of opinion with regard to novelty, inventive step and industrial applicability</td></tr> <tr><td>IV</td><td><input type="checkbox"/></td><td>Lack of unity of invention</td></tr> <tr><td>V</td><td><input checked="" type="checkbox"/></td><td>Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement</td></tr> <tr><td>VI</td><td><input type="checkbox"/></td><td>Certain documents cited</td></tr> <tr><td>VII</td><td><input type="checkbox"/></td><td>Certain defects in the international application</td></tr> <tr><td>VIII</td><td><input type="checkbox"/></td><td>Certain observations on the international application</td></tr> </table> </li> </ol>	I	<input checked="" type="checkbox"/>	Basis of the report	II	<input type="checkbox"/>	Priority	III	<input type="checkbox"/>	Non-establishment of opinion with regard to novelty, inventive step and industrial applicability	IV	<input type="checkbox"/>	Lack of unity of invention	V	<input checked="" type="checkbox"/>	Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement	VI	<input type="checkbox"/>	Certain documents cited	VII	<input type="checkbox"/>	Certain defects in the international application	VIII	<input type="checkbox"/>	Certain observations on the international application
I	<input checked="" type="checkbox"/>	Basis of the report																						
II	<input type="checkbox"/>	Priority																						
III	<input type="checkbox"/>	Non-establishment of opinion with regard to novelty, inventive step and industrial applicability																						
IV	<input type="checkbox"/>	Lack of unity of invention																						
V	<input checked="" type="checkbox"/>	Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement																						
VI	<input type="checkbox"/>	Certain documents cited																						
VII	<input type="checkbox"/>	Certain defects in the international application																						
VIII	<input type="checkbox"/>	Certain observations on the international application																						

Date of submission of the demand  <b>06.12.2000</b>	Date of completion of this report  <b>18.10.2001</b>
Name and mailing address of the IPEA/SE Patent- och registreringsverket Box 5055 S-102 42 STOCKHOLM Facsimile No. 08-667 72 88	Authorized officer  <b>Monika Bohlin/Els</b> Telephone No. 08-782 25 00

## INTERNATIONAL PRELIMINARY EXAMINATION REPORT

International application No.

PCT/SE00/01109

## I. Basis of the report

## 1. With regard to the elements of the international application:\*

- ☒ the international application as originally filed
- ☐ the description: \_\_\_\_\_, as originally filed  
pages \_\_\_\_\_, filed with the demand  
pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the claims: \_\_\_\_\_, as originally filed  
pages \_\_\_\_\_, as amended (together with any statement) under article 19  
pages \_\_\_\_\_, filed with the demand  
pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the drawings: \_\_\_\_\_, as originally filed  
pages \_\_\_\_\_, filed with the demand  
pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_
- ☐ the sequence listing part of the description: \_\_\_\_\_, as originally filed  
pages \_\_\_\_\_, filed with the demand  
pages \_\_\_\_\_, filed with the letter of \_\_\_\_\_

2. With regard to the language, all the elements marked above were available or furnished to this Authority in the language in which the international application was filed, unless otherwise indicated under this item.  
These elements were available or furnished to this Authority in the following language \_\_\_\_\_ which is:

- ☐ the language of a translation furnished for the purposes of international search (under Rule 23.1(b)).
- ☐ the language of publication of the international application (under Rule 48.3(b)).
- ☐ the language of the translation furnished for the purposes of international preliminary examination (under Rules 55.2 and/or 55.3).

## 3. With regard to any nucleotide and/or amino acid sequence disclosed in the international application, the international preliminary examination was carried out on the basis of the sequence listing:

- ☐ contained in the international application in written form.
- ☐ filed together with the international application in computer readable form.
- ☐ furnished subsequently to this Authority in written form.
- ☐ furnished subsequently to this Authority in computer readable form.
- ☐ The statement that the subsequently furnished written sequence listing does not go beyond the disclosure in the international application as filed has been furnished.
- ☐ The statement that the information recorded in computer readable form is identical to the written sequence listing has been furnished.

4. ☐ The amendments have resulted in the cancellation of:

- ☐ the description, pages \_\_\_\_\_
- ☐ the claims, Nos. \_\_\_\_\_
- ☐ the drawings, sheet/fig \_\_\_\_\_

5. ☐ This report has been established as if (some of) the amendments had not been made, since they have been considered to go beyond the disclosure as filed, as indicated in the Supplemental Box (Rule 70.2 (c)).\*\*

\* Replacement sheets which have been furnished to the receiving Office in response to an invitation under Article 14 are referred to in this report as "originally filed" and are annexed to this report since they do not contain amendments (Rules 70.16 and 70.17).

\*\* Any replacement sheet containing such amendments must be referred to under item I and annexed to this report.



## INTERNATIONAL PRELIMINARY EXAMINATION REPORT

International application No.

PCT/SE00/01109

## V. Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement

## 1. Statement

Novelty (N)	Claims	<u>1-20</u>	YES
	Claims		NO
Inventive step (IS)	Claims	<u>1-20</u>	YES
	Claims		NO
Industrial applicability (IA)	Claims	<u>1-20</u>	YES
	Claims		NO

## 2. Citations and explanations (Rule 70.7)

## Cited documents:

D1 US 4741015 A  
D2 WO 8908269 A1  
D3 US 5751781 A  
D4 FR 2529088 A1  
D5 GB 1129653 A

The documents cited in the International Search Report represent background art.

The invention defined in claims 1-20 is not disclosed in any of these documents.

None of the cited documents gives any indication towards the claimed radiation gantry. No relevant combination of the cited documents would lead a person skilled in the art to the invention defined in the claims.

Therefore, the invention defined in claims 1-20 is novel and is considered to involve an inventive step. It is also considered to be industrially applicable.

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/01109

## A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61N 5/01, A61B 6/04

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61N, A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4741015 A (PIERRE CHARRIER), 26 April 1988 (26.04.88), column 1, line 6 - line 60; column 2, line 40 - column 3, line 4, figures; abstract --	1-20
A	WO 8908269 A1 (ANALOGIC CORPORATION), 8 Sept 1989 (08.09.89), figures; claims; abstract --	1-20
A	US 5751781 A (KEVIN J. BROWN ET AL), 12 May 1998 (12.05.98), figures; claims; abstract --	1-20

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

4 October 2000

Date of mailing of the international search report

10-10-2000

Name and mailing address of the ISA/

Swedish Patent Office

Box 5055, S-102 42 STOCKHOLM

Facsimile No. +46 8 666 02 86

Authorized officer

Monika Bohlin/MP

Telephone No. +46 8 782 25 00

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/SE 00/01109

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	FR 2529088 A1 (MECANIQUE ET CONCEPTIONS INDUSTRIELLES MODERNES (MCIM)), 30 December 1983 (30.12.83), page 2, line 21 - page 4, column 16, figures; claims --	1-20
A	GB 1129653 A (ARTASHES ERVANDOVICH ATOVMIAN ET AL), 9 October 1968 (09.10.68), page 1, line 24 - line 82; page 3, line 24 - line 58, figures; claims -- -----	1-20

**INTERNATIONAL SEARCH REPORT**  
Information on patent family members

01/08/00

International application No.  
PCT/SE 00/01109

Patent document cited in search report			Publication date	Patent family member(s)	Publication date
US	4741015	A	26/04/88	NONE	
WO	8908269	A1	08/09/89	DE 3855460 D,T	02/01/97
				DE 3856008 D,T	15/01/98
				DE 3856009 D,T	15/01/98
				DE 3856010 D,T	08/01/98
				DE 3887333 D,T	19/05/94
				EP 0357732 A,B	14/03/90
				EP 0579032 A,B	19/01/94
				EP 0579033 A,B	19/01/94
				EP 0579034 A,B	19/01/94
				EP 0579035 A,B	19/01/94
				JP 2503282 T	11/10/90
				JP 2847655 B	20/01/99
				US RE34379 E	14/09/93
				US RE36099 E	16/02/99
				US 4928283 A	22/05/90
US	5751781	A	12/05/98	GB 2305975 A	23/04/97
				GB 9520567 D	00/00/00
				EP 0814869 A	07/01/98
				JP 10511595 T	10/11/98
				WO 9713552 A	17/04/97
FR	2529088	A1	30/12/83	NONE	
GB	1129653	A	09/10/68	DE 1516402 B	15/01/70
				FR 1454127 A	22/12/66

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
14 December 2000 (14.12.2000)


PCT

(10) International Publication Number  
WO 00/74779 A1

- (51) International Patent Classification<sup>7</sup>: A61N 5/01, A61B 6/04 (74) Agents: HEDBERG, Åke et al.; Aros Patent AB, P.O. Box 1544, S-751 45 Uppsala (SE).
- (21) International Application Number: PCT/SE00/01109 (81) Designated States (*national*): AE, AG, AL, AM, AT, AT (utility model), AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, CZ (utility model), DE, DE (utility model), DK, DK (utility model), DM, DZ, EE, EE (utility model), ES, FI, FI (utility model), GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KR (utility model), KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (22) International Filing Date: 30 May 2000 (30.05.2000)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data: 9902163-6 9 June 1999 (09.06.1999) SE
- (71) Applicant (*for all designated States except US*): SCANDITRONIX MEDICAL AB [SE/SE]; Stålgatan 14, S-754 50 Uppsala (SE).
- (72) Inventor; and (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).
- (75) Inventor/Applicant (*for US only*): NÄFSTADIUS, Peder [SE/SE]; Palissadgränd 66, S-187 66 Täby (SE).

[Continued on next page]

(54) Title: STABLE ROTATABLE RADIATION GANTRY

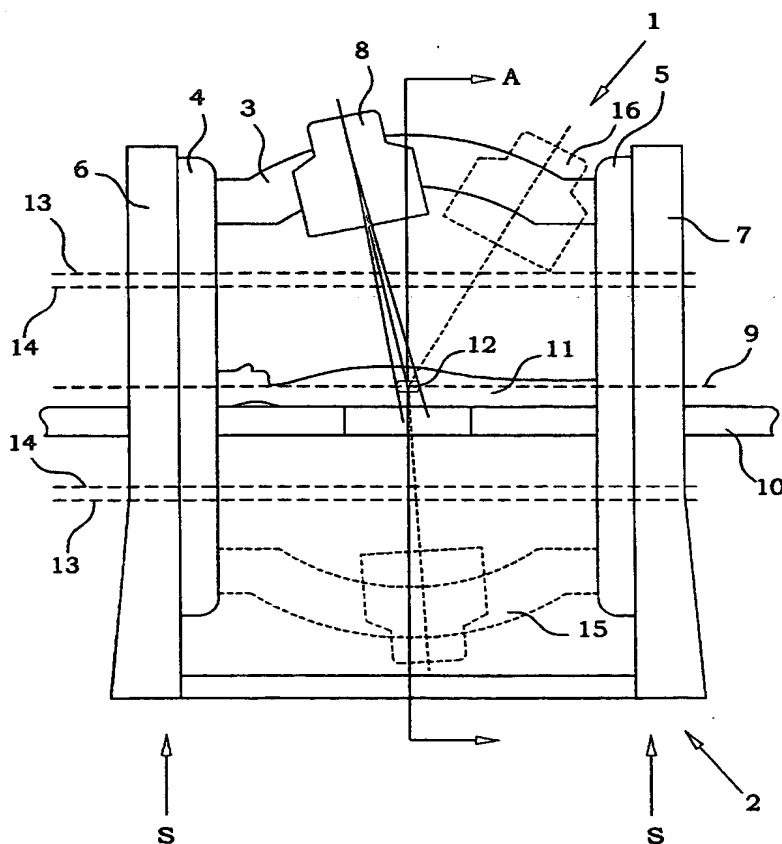

(57) Abstract: The present invention presents an irradiation device providing a free volume around the longitudinal axis of the body (13) around the body to be irradiated. The supporting parts of a gantry (1, 2) are situated substantially radially with respect to the longitudinal axis. The gantry comprises an inner gantry part (1) with at least two supporting locations (S) to an outer gantry portion (2). The support locations (S) are situated at each side of a treatment volume (12). A radiation head (8), mechanically attached to the inner gantry part (1) and arranged to direct radiation to the treatment volume (12) is movable around the treatment volume (12). In preferred embodiments, the parts (20, 21, 22, 23) of the gantry are formed as rings, leaving a free space along the rotational axis (9). A body-supporting couch (10) is arranged along the rotational axis extending through the hollow parts (20, 21, 22, 23). The radiation head (8) is preferably movable in a path also perpendicular to the rotation axis (9). Non-coplanar treatments are thereby possible to obtain. The arrangements are suitable for applying numerical control of the gantry movements. The invention also discloses irradiation methods suitable for such devices.

WO 00/74779 A1



**Published:**

- *With international search report.*
- *Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.*

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

## STABLE ROTATABLE RADIATION GANTRY

### TECHNICAL FIELD

5 The present invention relates to devices and methods for irradiation and in particular to devices and methods for irradiation in more than one direction.

### BACKGROUND

10 Radiation, in the form of electromagnetic radiation or particle radiation, is today used for many purposes, e.g. modification of properties of materials, sterilising purposes as well as medical diagnostics and treatment. The different purposes put different requirements on the methods and devices used, but there are also big similarities.

15 In the field of radiotherapy and radiosurgery treatment, a common general method is to arrange a patient on a couch. A radiation head is directed relative the patient in order to direct radiation to a certain treatment volume, e.g. a tumour. The general requirement in such applications is to maximise  
20 the dose within the treatment volume, while minimise the dose in tissue material outside the treatment volume. One way to accomplish this is to irradiate the treatment volume from different directions, whereby the treatment volume receives a radiation dose at all instances, while certain parts of the surrounding material only receives doses at some occasion.

25 There are different ways to accomplish multi-directional radiation. For small radiation sources, a multitude of sources may be used. This may e.g. be used for Co-60 sources, which normally are limited in size and weight. For other radiation sources, which are heavier and/or larger, this solution  
30 becomes unpractical. Another approach is instead to arrange the radiation head in a movable fashion, e.g. attached to a gantry, which is allowed to move. Since radiation heads often are very heavy, in some cases up to several thousand kilograms, the gantries have typically to be build extremely

stable. The easiest way to move the gantry is in such cases to use a rotating movement. Since it in most applications is desirable to have the body to be irradiated positioned horizontally, the rotation axis is typically oriented horizontally, so that the gantry is allowed to move besides and under the body.

The gantry according to prior art is typically designed in a general L or C shape, and the rotational support is provided at one axial end of the body. However, the heavy weights may cause the gantry arms to elastically deform, which results in a modified rotational motion. Instead of a pure rotation, the gantry will precess, creating an inaccuracy in the positioning of the radiation head. Furthermore, the heavy loads will apply extreme forces on the rotation bearings, even if many attempts of balancing the gantries have been made. Due to these reasons, the gantry movements are limited in speed, since high accelerations and retardations increase the load even further.

The couches used together with this type of gantries is typically designed with a support portion, which is situated outside the area of the gantry movement, and a couch sticking into the gantry region substantially horizontally. The reason for this is that no couch supports can be placed in the path of the gantry rotation. Due to the asymmetric design, the couches are typically very sensitive for the positioning of the body on the couch. Placing a body on the couch will typically cause a displacement of up to 1 cm, and changing the location of the body on the couch may alter the displacement several millimetres. This implies that the motion of the couch can not be used during an accurate treatment of e.g. a tumour in the treatment volume.

Since the radiation treatment is intended to be performed also from below, it is important that the couch close to the treatment volume do not absorb the radiation and causes any production of secondary radiation. One way to solve this is to remove most of the solid material from the couch close to the treatment volume, and only leave e.g. a thin stretched foil of material with



low cross section for the used radiation. However, in order to support body weight on both sides of the treatment volume, some stiff solid constructions, connecting solid parts of the couch, have to pass relatively close to the treatment volume, e.g. in the form of C-arms or beams. However, changing the irradiation direction, may lead to collisions with such arms, which has to be movable, depending on the position of the radiation head.

Using gantries with a single rotational movement allows for irradiation in different directions in one and the same plane, so called coplanar irradiation. If the ratio between the doses of the treatment volume and the tissues outside, respectively, is going to be increased further, radiation in directions outside this irradiation plane has to be accomplished, so called non-coplanar irradiation. A trivial solution could be to provide the gantry with several radiation heads, irradiating the treatment volume in different out-of-plane directions. However, expensive or heavy radiation heads are not suitable for such solutions.

There are several attempts for solutions giving non-coplanar irradiation in prior art. Some uses radiation deviation means, or uses the possibility to tilt the body to be irradiated. Deviation means are, however, often difficult to control in an exact way, in particular when constant radiation beam properties are concerned. Tilting of the body is unsuitable due to risks of displacements, between the body and the couch, of the couch itself as well as displacements within the body.

The British patent GB 1,129,653 discloses a device for radiation therapy, which is movable in several directions. It discloses the possibility to rotate a gantry around a horizontal axis and at the same time displace the radiation head along a perpendicular circular arch relative to the gantry. This solution provides non-coplanar irradiation, but still performs the problems with instability in the gantry and couch.

The American patent US 5,577,094 discloses another solution, where the gantry is movable along two perpendicular circular paths. This is, besides the earlier described stability problems also restricted mainly to cranial treatments, since the available space around the treatment volume substantially is restricted to one side.

A common problem with most equipment according to the state of the art is that there is a risk for collision between the radiation head and the body, to be irradiated, or couch. When changing irradiation directions, a manual inspection is normally required during movements of the radiation head and/or gantry to ensure that the body is not jammed between the couch and the gantry. This problem makes any requested automation of the treatment difficult. There are some solutions of this problem, which are based on contact switches, which stops any movement, if any distances become too small. Normally, this is combined with using friction safety clutches, applied to the gantry movement. When using such solutions, the maximum allowed moment on the gantry is reduced, which further reduces the maximum retardation and acceleration. Furthermore, the contact switch solution has some reaction time, which put restrictions on the maximum speed of any motion.

The international patent application WO 89/08269 discloses an X-ray tomography apparatus. The apparatus is mounted for rotation around a patient within a circular frame. The apparatus can be displaced along the patient irradiating parallel sections of the body. However, facilities for non-coplanar irradiation are neither discussed nor easily provided for in this apparatus.

## SUMMARY

It is therefore a general object of the present invention to provide irradiation devices, which do not present the problems discussed above. In more detail, it is an object of the present invention to provide irradiation devices, which

presents an improved stability in the gantry and couch. A further object with the present invention is to provide irradiation devices, which can provide accurate non-coplanar irradiation without involving movement of the body to be irradiated. Another object of the present invention is to provide a design of irradiation devices, which simplifies automatic control of the movements of different parts, without risk for collisions. Yet another object of the present invention is to provide irradiation devices which can provide radiation continuously over an angle considerably exceeding a full turn.

The above objects are achieved by a device and a method according to the enclosed claims. In general, the objects of the present invention are achieved by providing an irradiation device providing a free volume around the body to be irradiated, along its entire longitudinal axis. The supporting parts of a gantry of the irradiation device are situated substantially radially with respect to the free volume. The gantry comprises an inner gantry part with at least two supporting locations to an outer gantry part. The support locations are situated at each side of a treatment volume. A radiation head, mechanically attached to the gantry and arranged to direct radiation to the treatment volume is movable around the treatment volume. In preferred embodiments, parts of the inner and outer gantry parts are formed as rings, leaving a free space along the longitudinal axis of the body. A body-supporting couch is arranged along the rotational axis and through the hollow gantry parts. The radiation head is preferably movable along a path also perpendicular to the rotation axis. Non-coplanar treatments are thereby possible to obtain. The arrangements are suitable for applying numerical control of the gantry movements.

## BRIEF DESCRIPTION OF THE DRAWINGS

The invention, together with further objects and advantages thereof, may best be understood by referring to the following description taken together with the accompanying drawings, in which:

FIG. 1 is a side view of a first embodiment of an irradiation device according to the present invention;

FIG. 2 is a sectional view of the irradiation device of fig. 1, taken along the line A-A;

FIG. 3a is a perspective view of a couch to be used with an irradiation device according to the present invention;

FIG. 3b illustrates the movement region required for the couch;

FIG. 4 is a schematic drawing illustrating the irradiation directions achievable by a device according to the first embodiment of the present invention;

FIG. 5 is a side view of a second embodiment of an irradiation device according to the present invention;

FIG. 6 is a sectional view of the irradiation device of fig. 7, taken along the line B-B;

FIG. 7 is a schematic drawing illustrating the irradiation directions achievable by a device according to the second embodiment of the present invention;

FIG. 8 is a side view of a third embodiment of an irradiation device according to the present invention;

FIG. 9 is a sectional view of the irradiation device of fig. 8, taken along the line C-C;

FIG. 10 is a schematic drawing illustrating the irradiation directions achievable by a device according to the third embodiment of the present invention;

FIG. 11 is a side view of a fourth embodiment of an irradiation device according to the present invention; and

FIG. 12 is a side view of the embodiment of Fig. 11 used in a coplanar section mode.

## DETAILED DESCRIPTION

The present invention is based on some general more or less pure geometrical considerations. The stability problems for gantries and couches

according to the state of the art are based on the alignment of the gantry support and the couch. The gantry is normally placed substantially in the vicinity of the axis of rotation, which is substantially aligned with the extension of the couch. The couch is only possible to support in one end due to the interference with the gantry movements and the unstable gantry design is based on requirements not to disturb the couch more than necessary.

In the present invention, the geometric considerations are changed. In order to make it possible to provide a stable couch design, a volume around the couch, comprising the volume in which the body to be irradiated is placed, is reserved for couch parts only. No gantry parts are allowed to be present within this volume. All movable parts of the gantry are in all possible situations situated at a distance from the rotation axis of the radiation head which is larger than a predetermined value. The free volume is extended along the couch axis through the entire gantry arrangement. The gantry is supposed to be movable around this reserved volume, irradiating the body from different directions.

As a result of this volume reservation, the gantry is no longer allowed to be placed axially with respect to the couch, the body and the rotation axis. The gantry supporting parts thus have to be moved from an axial position to a radial position, with respect of the couch. That means that the supporting means of the gantry has to be placed substantially above, below or at the sides of the couch.

The gantry design has to be stable, but at the same time allow for examination of the body to be treated. Since the gantry, in a radial position with respect to the body, occupies the same volumes that are used for e.g. visual or manual examination of the body, the gantry thus has to be kept relatively small in size. This complicates the stability problems even more. According to the present invention, the stability of the gantry is achieved by arranging an inner gantry part with two supporting locations relative to an

outer gantry part. These two supporting locations are placed at each side of the treatment volume, i.e. the volume of the body that is to be irradiated. Since there are two support locations, the stability of the gantry is increased, without increasing the volume or inherent strength of the gantry. The two support locations may be placed in any direction, radially or axially, as long as the free volume around the couch is preserved.

Below, four embodiments of the present invention are described, which illustrates devices where the supporting locations of the inner gantry part to the outer gantry part are placed in different directions relative to the treatment volume. The invention is particularly useful for radiotherapy and radiosurgery applications. However, as anyone skilled in the art understands, there are other modifications and alternative embodiments, which still are covered by the scope of the invention.

In fig. 1, a side view of a first embodiment of an irradiation device according to the invention is illustrated. A radiation head 8 is mechanically supported by an inner gantry part, generally denoted by 1. The inner gantry part 1 comprises in the present embodiment a circle arc portion 3, a first ring portion 4 and a second ring portion 5. The radiation head 8 is movable along the circle arc portion 3, and arranged to direct radiation to a treatment volume 12. A body 11 is placed at a body-supporting couch, generally denoted by 10. The treatment volume 12 is thereby in the normal case a part of the body 11, which is going to be treated by the radiation emitted from the radiation head 8. The first ring portion 4 and a second ring portion 5 are in this embodiment positioned at each side of the treatment volume 12. The ring portions 4, 5 are rotatably supported by an outer gantry part 2, comprising a first support portion 6 and a second support portion 7. Accordingly, the inner gantry part 1 is provided with two supporting locations S with respect to the outer gantry part 2. The inner gantry part 1 is by this arrangement possible to rotate around a rotation axis 9, which is substantially horizontal. In the present invention, the two supporting locations S are situated on each side of the treatment volume 12, in an axial

direction, i.e. in the direction of the rotation axis 9. The treatment volume 12 is in a preferred embodiment positioned at the rotation axis 9.

The inner gantry part 1 is rotatable around the rotation axis 9, and may thus be used also to irradiate the treatment volume 12 from below, as indicated by the broken line structure 15. The radiation head 8 is movable along the circle arc portion 3 and the broken line head 16 illustrates one end position for the radiation head 8. The motion of the inner gantry part 1 and the radiation head 8 between the supporting locations S of the inner gantry part 1 always takes place outside a cylindrical volume, which is indicated by the broken line 13. No movable parts of the inner gantry part 1 will ever exist within this gantry rotational envelope 13, independent of the intended motion of the radiation head 8. The gantry rotational envelope 13 thus constitutes the free volume around the body to be treated 11. The body to be treated 11 and the couch 10 are both preferably enclosed within a second cylindrical volume, a body positioning volume 14. This body positioning volume 14 is totally enclosed by the gantry rotational envelope 13, preferably with a certain security margin. In such a case, there is no risk for jamming of the body 11 against the couch 10 or destruction of the radiation head 8 against the couch 10 at any time. This implies that the couch 10 can not have any supporting portions against e.g. floor or ceiling in the space between the supporting locations S of the inner gantry part 1.

A preferable solution of the couch-supporting problem is illustrated in fig. 2, where the irradiation device of fig. 1 is illustrated in a sectional view along the line A-A in the axial direction. The ring portions 4, 5 of the inner gantry part 1 are designed with a substantially circular shape, defining rotationally symmetric outer surfaces. These rotationally symmetric outer surfaces form the bearing locations of the inner gantry part 1. The support portions 6, 7 are in a corresponding manner designed with rotationally symmetric inner surfaces. The support portions 6, 7 are adapted to fit the ring portions 4, 5, leaving appropriate space for bearings, in the form of e.g. roller bearings. Since the ring portions 4, 5 and the support portions 6, 7 are formed without

any parts along the rotation axis 9, there is free space available. The couch may thus extend through the ring portions 4, 5 and the support portions 6, 7, along the rotation axis 9. The couch 10 may therefore be supported by the outer gantry part 2 or, as shown in the figure, by separate supports outside the inner gantry part bearing locations. In this embodiment, the couch support is movable in height and horizontally, perpendicular to the rotation axis 9. This two-dimensional mobility is accomplished by means in the couch supports. In fig. 2, a slot portion 20 allowing for horizontal movement, and a piston 18 and cylinder 19 for vertical movement are shown. The couch 10 and its supports are described more in detail below.

Fig. 3a illustrates a perspective view of a preferred embodiment of a couch 10 according to the present invention. The couch comprises a first couch support portion 21 and a second couch support portion 22. As discussed above, the couch support portions 21, 22 may be integrated in the gantry support or provided as separate means. From the first couch support section 21, a first rigid couch portion 23 extends towards the treatment volume. From the second couch support portion 22, a second rigid couch section 24 extends towards the treatment volume, in the opposite direction. The front parts of the rigid couch sections 23, 24 are placed apart from each other and thereby form an empty volume 29 there between. This empty volume 29, at operation of the irradiation device, is situated just beneath the treatment volume 12 (see fig. 1). The rigid sections 23, 24 are preferably interconnected by a thin foil 25 of material with a low radiation cross section, e.g. polyethylene. The foil 25 is in this embodiment provided as an endless belt, which is driven by two rolls, 26, 27, and may thus serve for changing the position of the body along the rotation axis. Alternatively, rigid plates of e.g. carbon fibre may be used instead of the thin foil.

The rigid sections 23, 24 are in a preferred embodiment movable relative the gantry. Preferably, the displacements are possible in at least two translation directions, vertically, and horizontally and perpendicular to the rotation axis 9, respectively. According to fig. 3a, these directions are denoted z and y,



respectively. The y-motion of the rigid sections 23, 24 is in the present embodiment accomplished by letting a protrusion 28 of the rigid sections 23, 24 slide in a slot portion 20. Any conventional means for causing and controlling this motion may be used. The z-motion of the rigid sections 23, 24 is in the present embodiment accomplished by a piston 18 of the couch support portions 21, 22 which can be moved up and down in a cylinder 19. In a preferred embodiment, the motion of the rigid sections 23, 24 are independent of each other, which provides for various positioning possibilities for the body. As indicated above, the foil 25 may be used for changing the position of a body on the couch 10 in the x-direction, by driving the endless belt by the two rolls 26 and 27.

Fig. 3b illustrates a cross section of a body to be irradiated. The motion possibilities of the couch should be such that all parts of the body would be possible to position at the treatment volume. The limit movements in the z and y directions should therefore enclose the body volume, or at least the parts of the body volume, which may be a target for irradiation.

Now referring again to fig. 1 and fig. 2, the co-operation between the couch and the gantry is easily understood. The inner gantry part 1 is rotatably supported by the outer gantry part 2. The couch 10 extends from both ends along the rotation axis 9, leaving the open space 24 beneath the treatment volume 12. The couch support portions 21, 22 are provided outside the inner gantry part support locations S. When the inner gantry part 1 is rotated around the couch 10, the treatment volume 12 is available from all directions without any radiation disturbing material, except for the thin stretched foil 25.

It is easily seen in fig. 1 and 2, that the gantry is supported mainly in the radial direction, with respect of the rotation axis 9. The circular design of the ring portions 4, 5 and the support portions 6, 7 enables the clearance of the volume around the couch 10. It is also seen that since the centre of mass of

the inner gantry part 1 always is situated between the support locations S, there are relatively low bending moment present in the gantry.

In a preferred embodiment, the inner gantry part 1 is continuously rotatable, relative the outer gantry part 2. The mechanical operation and support is easily provided with e.g. conventional gear solutions and bearings. One limiting factor in equipment existing today is the wiring for the radiation head. However, by introducing sliding contacts between the inner gantry part 1 and the outer gantry part 2, preferably in connection with the mechanical bearing, a true continuous rotational motion may be achieved.

Returning to fig. 1, the radiation head 8 is movable along a circle arc portion 3 of the inner gantry part 1. The circle arc portion 3 has a centre of curvature, which is situated within the treatment volume 12, and preferably on the rotation axis 9. When the radiation head 8 is moved along the circle arc portion 3, it maintains the radiation direction towards the treatment volume 12. By combining the rotation around the horizontal axis 9 and the motion along the circle arc portion 3, a multitude of irradiation directions may be reached. During such movements, the radiation head 8 is situated at the same distance from the treatment volume 12.

The treatment situation is schematically illustrated in fig. 4. The radiation head 8 is possible to move anywhere along a spherical surface, which is cut by two parallel vertical planes 30, 31, perpendicular to the rotation axis 9. All directions within an angle  $V1$  from a centre vertical plane 32 are achievable. A non-coplanar treatment may be achieved. Other angles than perpendicular to the rotation axis may be of interest to use in order to avoid damage of vital organs situated in the vicinity of the treatment volume 12. If the radiation head 8 is fixed at a certain position along the circle arc portion 3 and the inner gantry portion 1 is rotated, the irradiation of the treatment volume 12 will be applied in a conical shape. If the displacement the radiation head 8 is controlled simultaneously as the inner gantry part 1 moves, any other geometrical irradiation pattern may be accomplished. In

this way an irradiation path on the treatment volume may be adapted to each individual case, depending on the nature of the target and the sensitivity for radiation damage in the surroundings of the treatment volume 12.

5

10

The possibility of continuous rotation together with the possibility to change the angle of the radiation head perpendicular to the rotation axis facilitates different treatment possibilities. If several non-coplanar irradiation paths are to be performed, the paths may be scheduled without taking any limitations in the rotation into account. The path may e.g. be selected as a continuous spherical shaped coil around the treatment volume 12.

15

20

The above treatments are preferably performed in an automated manner. Since the irradiation devices according to the present invention almost totally removes the risks for mechanical jamming or contact destruction, the operational processes may be automated easily. The possibility to spread the radiation dose over a larger volume around the treatment volume is used more efficiently, if short exposures from a multitude of directions are given. This requires a rapid movement of the radiation head, which is facilitated by the stable gantry construction according to the present invention. Furthermore, since the gantry construction according to the present invention reduces the risk for jamming considerably, other approaches of control may be implemented.

25

30

The motion of the radiation head in the two perpendicular directions may preferably be performed utilising numerical control procedures. In such a system, the coordinates of the radiation head may easily be controlled together with e.g. radiation intensity, radiation distribution etc. in order to tailoring a radiation treatment. Revolution times of the inner gantry part of the order of 5 s would be possible, enabling the radiation head to move between two arbitrary selected positions in times of the same order of magnitude.

The motion of the couch may also be controlled automatically. However, there is a general request not to move the body during treatment, so the main purposes for automatic control of the couch movement is to facilitate the introduction of the body into the area of the treatment volume.

5 In fig. 5, a side view of a second embodiment of an irradiation device according to the invention is illustrated. In fig. 6 the irradiation device of fig. 5 is illustrated in a sectional view along the line B-B in the axial direction. A radiation head 8 is mechanically supported by an inner gantry part, generally denoted by 1. The inner gantry part 1 comprises in the present  
10 embodiment a head supporting arm 213, a ring portion 201 and a counterweight 206. The radiation head 8 is fixed at the head supporting arm 213, and arranged to direct radiation to a treatment volume 12. A body 11 is placed at a body-supporting couch, generally denoted by 10. The treatment  
15 volume 12 is thereby in the normal case a part of the body 11, which is going to be treated by the radiation emitted from the radiation head 8. The head supporting arm 213 is movable along the ring portion 201, which means that the radiation head is able to rotate around a rotation axis 9, which is substantially horizontal. The treatment volume 12 is in a preferred  
20 embodiment positioned at the rotation axis 9.

The inner gantry part 1 is supported, via a first rotational support 204 and a second rotational support 205, by an outer gantry part 2. The outer gantry part 2 comprises in this embodiment a generally C-shaped jaw portion 207,  
25 and a support portion 209. The jaw portion 207 surrounds the treatment volume 12 and is rotationally attached in its back end to the support portion by a rotational connection 208. The first rotational support 204 and the second rotational support 205 are attached to the front ends 202 and 203, respectively, of the jaw portion 207, and are therefore positioned at each side  
30 of the treatment volume 12, in the vertical direction. Accordingly, the inner gantry part 1 is provided with two supporting locations S with respect to the outer gantry part 2. The supporting locations S are situated on each side of the treatment volume 12, in a radial direction.

The radiation head 8 is rotatable around the rotation axis 9, and may thus be used also to irradiate the treatment volume 12 from below. In order to reach non-coplanar irradiation directions, the inner gantry part 1 is rotated, either around a vertical axis 210 by the first and second rotational supports 204, 205, or around a horizontal axis 211 by the rotational connection 208. A slight rotation of the inner gantry part 1 will put the ring portion 201 as indicated by the broken line ring 212. Such a tilting will thus limit the free space around the couch 10 and body 11, and a restriction of this tilting is necessary to ensure a free space around the body. The first and second rotational supports 204, 205 are situated in the same plane as the radiation head 8, while the ring portion 201 is slightly offset, as clearly seen in fig. 5. The axes of the tilting of the inner gantry part 1, either the vertical axis 210 or the horizontal axis 211, are intersecting the treatment volume 12. This means that the radiation head 8 always is directed substantially towards the treatment volume 12.

The tilting of the inner gantry part 1 and the radiation head 8 is restricted in such a manner that all parts of the gantry and radiation head 8 are located outside a cylindrical volume, which is indicated by the broken line 13. No movable parts of the inner gantry part 1 will ever exist within this gantry rotational envelope 13, independent of the intended motion of the radiation head 8 or tilting of the inner gantry part 1. The gantry rotational envelope 13 thus constitutes the free volume around the body to be treated 11. The body to be treated 11 and the couch 10 are as in previous embodiment both preferably enclosed within a second cylindrical volume, a body positioning volume 14. This body positioning volume 14 is totally enclosed by the gantry rotational envelope 13, preferably with a certain security margin. In such a case, there is no risk for jamming of the body 11 against the couch 10 or destruction of the radiation head 8 against the couch 10 at any time.

The ring portion 201 of the inner gantry part 1 is designed with a substantially circular shape. This means that the ring portion 201 is formed

without any parts along the rotation axis 9, where free space is available. The couch 10 may thus extend through the ring portion 201, substantially along the rotation axis 9. When the ring portion 201 is tilted in any direction, the rotation axis 9 of the radiation head 8 is also tilted. However, since the tilting is restricted to relatively small angles, the angular deviation between the longitudinal axis of the couch and body, and the rotation axis, is also relatively small.

In fig. 5, it may be noticed, that since the first and second rotational supports 204, 205 are situated in the same plane as the radiation head 8 and the ring portion 201 is displaced from the axis 210, the ring portion 201 applies a torque on the outer gantry part 2, which would tend to rotate the rotational connection 208. In order to compensate for this torque, a counterweight 206, is attached to the ring portion 201. The counterweight 206 balances the weight of the ring portion 201. The counterweight 206 is fixed to the ring portion 201 and do not follow the rotation of the radiation head 8. This makes it possible to locate the counterweight in an area, which is not required for access to the body.

The treatment situation in a device according to the second embodiment of the present invention is schematically illustrated in fig. 7. The radiation head 8 is possible to move anywhere along a spherical surface, which is restricted by an angle  $V_2$  from the vertical axis and an angle  $V_3$  from the axis 211. All directions within these angles are achievable. A non-coplanar treatment may thus be achieved. Other angles than perpendicular to the rotation axis may be of interest to use in order to avoid damage of vital organs situated in the vicinity of the treatment volume 12. If the inner gantry part 1 is fixed at a certain position with respect to the outer gantry part 2, the rotational connection 208 is at a fixed angle and the radiation head 8 is rotated, the irradiation of the treatment volume 12 will be applied in a plane 33 defined by the axis 210. If the tilting of the gantry is controlled simultaneously as the radiation head 8 rotates, any other geometrical irradiation pattern may be accomplished. In this way an irradiation path on the treatment volume 12

may be adapted to each individual case, depending on the nature of the target and the sensitivity for radiation damage in the surroundings of the treatment volume 12.

5 It is easily seen in fig. 5 and 6, that the gantry is supported mainly in the radial direction, with respect of the longitudinal axis of the couch, and the rotation axis 9. The circular design of the ring portion 201 enables the clearance of the volume around the couch 10.

10 In fig. 8, a side view of a third embodiment of an irradiation device according to the invention is illustrated. In fig. 9 the irradiation device of fig. 8 is illustrated in a sectional view along the line C-C in the axial direction. A radiation head 8 is mechanically supported by an inner gantry part, generally denoted by 1. The inner gantry part 1 comprises in the present  
15 embodiment a ring portion 301. The radiation head 8 is arranged to direct radiation to a treatment volume 12. A body 11 is placed at a body-supporting couch, generally denoted by 10. The treatment volume 12 is thereby in the normal case a part of the body 11, which is going to be treated by the radiation emitted from the radiation head 8. The radiation head 8 is  
20 movable along the ring portion 301, which means that the radiation head 8 is able to rotate around a rotation axis 9, which is substantially horizontal. The treatment volume 12 is in a preferred embodiment positioned at the rotation axis 9.

25 The inner gantry part 1 is supported, via a first rotational support 304 and a second rotational support 305, by an outer gantry part 2. The outer gantry part 2 comprises in this embodiment a generally U-shaped jaw portion 307, and a support portion 309. The jaw portion 307 surrounds the treatment volume 12 and is rotationally attached in its lower part to the support  
30 portion 309 by a rotational connection 308. The first rotational support 304 and the second rotational support 305 are attached to the legs 302 and 303, respectively, of the jaw portion 307, and are therefore positioned at each side of the treatment volume 12, in a horizontal direction, perpendicular to the

longitudinal axis of the couch 10 and the body 11. Accordingly, the inner gantry part 1 is provided with two supporting locations S with respect to the outer gantry part 2. The supporting locations S are situated on each side of the treatment volume 12, in a radial direction.

5 The radiation head 8 is rotatable around the rotation axis 9, and may thus be used also to irradiate the treatment volume 12 from below. In order to reach non-coplanar irradiation directions, the inner gantry part 1 is rotated, either around a horizontal axis 310 by the first and second rotational  
10 supports 304, 305, or around a vertical axis 311 by the rotational connection 308. A slight rotation of the inner gantry part 1 will put the ring portion 301 as indicated by the broken line ring 312. Such a tilting will thus limit the free space around the couch 10 and body 11, and a restriction of this tilting is necessary to ensure a free space around the body. The first and  
15 second rotational supports 304, 305 are situated in the same plane as the radiation head 8 and the ring portion 301. The axes of the tilting of the inner gantry part 1, either the vertical axis 311 or the horizontal axis 310, are intersecting the treatment volume 12. This means that the radiation head 8 always is directed substantially towards the treatment volume 12.

20 The tilting of the inner gantry part 1 and the radiation head 8 is restricted in such a manner that all parts of the gantry and radiation head 8 are located outside a cylindrical volume, which is indicated by the broken line 13. No movable parts of the inner gantry part 1 will ever exist within this gantry  
25 rotational envelope 13, independent of the intended motion of the radiation head 8 or tilting of the inner gantry part 1. The gantry rotational envelope 13 thus constitutes the free volume around the body to be treated 11. The body to be treated 11 and the couch 10 are as in previous embodiments both preferably enclosed within a second cylindrical volume, a body positioning  
30 volume 14. This body positioning volume 14 is totally enclosed by the gantry rotational envelope 13, preferably with a certain security margin. In such a case, there is no risk for jamming of the body 11 against the couch 10 or destruction of the radiation head 8 against the couch 10 at any time.



The ring portion 301 of the inner gantry part 1 is designed with a substantially circular shape. This means that the ring portion 301 is formed without any parts along the rotation axis 9, where free space is available. The couch 10 may thus extend through the ring portion 301, substantially along the rotation axis 9. When the ring portion 301 is tilted in any direction, the rotation axis 9 of the radiation head 8 is also tilted. However, since the tilting is restricted to relatively small angles, the angular deviation between the longitudinal axis of the couch and body, and the rotation axis, is also relatively small.

In fig. 8, it may be noticed, that the radiation head 8 and the ring portion 201 are situated essentially in the same plane as the treatment volume 12. This means that the access to the treatment volume by visual or mechanical means is restricted. However, the design of the inner gantry part 1 is simplified as compared with the second embodiment, described above. In order to achieve access to the treatment volume, a similar design as in the previous embodiment may be provided, including weight balancing equipment.

The treatment situation in a device according to the second embodiment of the present invention is schematically illustrated in fig. 10. The radiation head 8 is possible to move anywhere along a spherical surface, which is restricted by an angle  $V5$  from the vertical axis 311 and an angle  $V5$  from a horizontal axis perpendicular to the longitudinal axis of the couch and body. All directions within these angles are achievable. A non-coplanar treatment may thus be achieved. Other angles than perpendicular to the rotation axis may be of interest to use in order to avoid damage of vital organs situated in the vicinity of the treatment volume 12. If the inner gantry part 1 is fixed at a certain position with respect to the outer gantry part 2, the rotational connection 308 is at a fixed angle and the radiation head 8 is rotated, the irradiation of the treatment volume 12 will be applied in a plane 34 defined by the axis 310. If the tilting of the gantry is controlled simultaneously as

the radiation head 8 rotates, any other geometrical irradiation pattern may be accomplished. In this way an irradiation path on the treatment volume 12 may be adapted to each individual case, depending on the nature of the target and the sensitivity for radiation damage in the surroundings of the treatment volume 12.

It is easily seen in fig. 8 and 9, that the gantry is supported mainly in the radial direction, with respect to the longitudinal axis of the couch, and the rotation axis 9. The circular design of the ring portion 301 enables the clearance of the volume around the couch 10. It is also seen that since the centre of mass of the inner gantry part 1 always is situated between the support locations S, there are relatively low bending moment present in the gantry.

In fig. 11, a fourth embodiment of an irradiation device according to the invention is illustrated. It is very similar to the first embodiment and corresponding parts having the same reference numbers will not be described or discussed again.

This fourth embodiment comprises a linear beam portion 17 interconnecting the first ring portion 4 and the second ring portion 5. The radiation head 8 is movable along the linear beam portion 17. In order to maintain the irradiation directed towards the treatment volume 12, the radiation head 8 is also allowed to be tilted with respect to the linear beam portion 17. This means that the relative angle between the linear beam portion 17 and the radiation head 8 is different in e.g. positions 15 and 16. In order to direct the radiation to the treatment volume 12, the direction of the radiation head 8 has to follow:

$$\alpha = \tan^{-1}\left(\frac{d}{r}\right) ,$$

where  $\alpha$  is the angle from the pure radial direction,  $d$  is the displacement of the radiation head 8, and  $r$  is the distance from the tilting axis of the radiation head to the rotation axis 9.

Furthermore, the radiation head 8 changes its distance to the treatment volume 12 when it moves along the linear beam portion 17. The distance varies as

$$s = \frac{r}{\cos \alpha} = \sqrt{r^2 + d^2} \quad ,$$

where  $s$  is the distance between the tilting axis of the radiation head 8 and the treatment volume. In most applications, it is advantageous if the isocenter distance is constant independent of the irradiation direction. However, one can compensate for the changing isocenter distance in this embodiment, by adapting collimator settings and dose according to e.g. the depth dose curve. Such adaptations may e.g. be included in the dose planning system.

Since the radiation head 8, in the embodiment of fig. 11, performs a linear motion, the mechanical construction of means for performing a radiation head motion can be simpler and thereby cheaper than corresponding means for a circular motion, such as in Fig. 1. The less complicated construction is a substantial advantage, since the radiation head 8 typically involves large weights. With the linear configuration, the centre of mass will remain stationary in the radial direction, cancelling the need for dynamic balance means. Any reduced complexity in the motion of the radiation head 8 may thus lead to substantial construction advantages.

However, the reduced complexity in the radiation head translation also leads to an increased complexity in that the radiation head 8 has to be tilted in a controlled manner depending on the translation position. However, means for tilting the radiation head 8 can be made rather simple, since the weight

of the radiation head 8 can be supported by separate means, e.g. by an axle, around which the radiation head 8 is tilted. The controlled tilting may e.g. be obtained by mechanical and/or electrical means according to conventionally available techniques.

Fig. 12 illustrates the embodiment of fig. 11 in an alternative operational mode. In this case an extended treatment volume 12 is demanded. The radiation head 8 can in such cases be moved along the linear beam portion 17 without tilting and without any focusing adjustment, e.g. to the positions 40. A series of coplanar irradiation are thus achieved, or alternatively, if the translation is continuous, a treatment along a helical path. Other variants of controlling the tilting and focusing are, of course, also possible. The embodiment of Fig. 11 and 12 may be advantageous for certain types of treatments, otherwise the embodiment of Fig. 1 is probably to prefer.

It will be understood by those skilled in the art that various modifications and changes may be made to the present invention without departure from the scope thereof, which is defined by the appended claims.

## CLAIMS

1. Irradiation device, comprising

a gantry (1-2);

5 a radiation head (8), mechanically supported by said gantry (1-2)  
and rotatable around a rotation axis (9);

said radiation head (8) is arranged to direct radiation to a treatment  
volume (12) situated substantially on said rotation axis (9);

10 and wherein all movable parts of said gantry (1-2) are, in all situations,  
situated at a distance from said rotation axis (9) which is larger than a  
predetermined value, **characterised in that** said gantry (1-2) comprises an  
inner gantry part (1) and an outer gantry part (2), said inner gantry part (1) is  
rotatably supported by said outer gantry part (2) at two support locations (S),  
situated at opposite sides of said treatment volume (12).

15 2. Irradiation device according to claim 1, **characterised in that** said gantry  
(1-2) is arranged substantially radially with respect of said treatment volume  
(12), as defined by said rotation axis (9).

20 3. Irradiation device according to claim 1 or 2, **characterised in that** said  
radiation head (8) is continuously rotatable around said rotation axis (9).

25 4. Irradiation device according to claim 1, 2 or 3, **characterised in that** said  
radiation head (8) is movable along at least one arc of a circle, substantially  
centred at said treatment volume (12), said arc being non-parallel with said  
rotation of said radiation head (8) around said rotation axis (9), whereby non-  
coplanar irradiation treatment is achievable.

30 5. Irradiation device according to any of the claims 1 to 4, **characterised in  
that** said inner gantry part (1) comprises a substantially circularly shaped  
portion (4, 5; 201; 301) arranged around said rotation axis (9).

6. Irradiation device according to any of the claims 1 to 5, characterised in that said support locations (S) are situated on opposite sides of said treatment volume (12), in the direction of said rotation axis (9).

5 7. Irradiation device according to claim 6, characterised in that said inner gantry part (1) comprises a first ring portion (4) and a second ring portion (5) separated in the direction of the rotation axis (9), said ring portions (4, 5) are carried in a first support portion (6) and a second support portion (7) of said outer gantry part (2), respectively.

10 8. Irradiation device according to claim 7, characterised in that at least one of said pairs of said ring portions (4, 5) and said support portion (6, 7) comprises electrical connections with sliding contacts.

15 9. Irradiation device according to claim 7 or 8, characterised in that said inner gantry part (1) further comprises an circle arc portion (3), on which said radiation head (8) is movably supported, whereby the centre of curvature of said arc portion (3) is situated in said treatment volume (12).

20 10. Irradiation device according to claim 7 or 8, characterised in that said inner gantry part (1) further comprises a linear beam portion (17), on which said radiation head (8) is movably supported.

25 11. Irradiation device according to claim 10, characterised in that said radiation head (8) is tiltably supported by said linear beam portion (17), said radiation head (8) directing its radiation towards said treatment volume (12) from any position relative to said linear beam portion (17).

30 12. Irradiation device according to any of the claims 1 to 5, characterised in that said support locations (S) are situated on opposite sides of said treatment volume (12), perpendicular to the direction of said rotation axis (9), and provide a tilting around a first tilting axis (210; 310) through said support

locations (S) and said treatment volume (12), whereby non-coplanar irradiation treatment is achievable.

13. Irradiation device according to claim 12, **characterised in that** said outer gantry part (2) comprises a rotational connection (208; 308), enabling a tilting of said inner gantry part (1) around a second tilting axis (211; 311) substantially perpendicular to the first tilting axis (210; 310); said second tilting axis (211; 311) goes substantially through said treatment volume (12).

14. Irradiation device according to claim 12 or 13, **characterised by** electrical connections with sliding contacts between said radiation head (8) and said inner gantry part (1).

15. Irradiation device according to any of the preceding claims, **characterised by** means for numerical control of movable parts in said irradiation device.

16. Irradiation device according to any of the preceding claims, **characterised in that** said irradiation device further comprises a body supporting couch (10), comprising two couch support portions (20, 21), situated on each side of said treatment volume (12), in the direction of said rotation axis (9).

17. Irradiation device according to claim 16, **characterised in that** said body supporting couch (10) is formed in two rigid parts (22, 23), each one attached to one respective of said couch support portions (20, 21), said rigid parts (22, 23) are interconnected by material (24) with a low radiation cross section.

18. Irradiation device according to claim 17, **characterised in that** said couch support portions (20, 21) are movable independently of each other.

19. Irradiation device according to claim 18, **characterised in that** said couch support portions (20, 21) are movable in two translational directions, substantially perpendicular to said rotation axis (9).

20. Irradiation device according to any of the claims 16 to 19, **characterized** in that said body-supporting couch (10) is arranged within a distance of said predetermined value from said rotation axis (9).



1/10

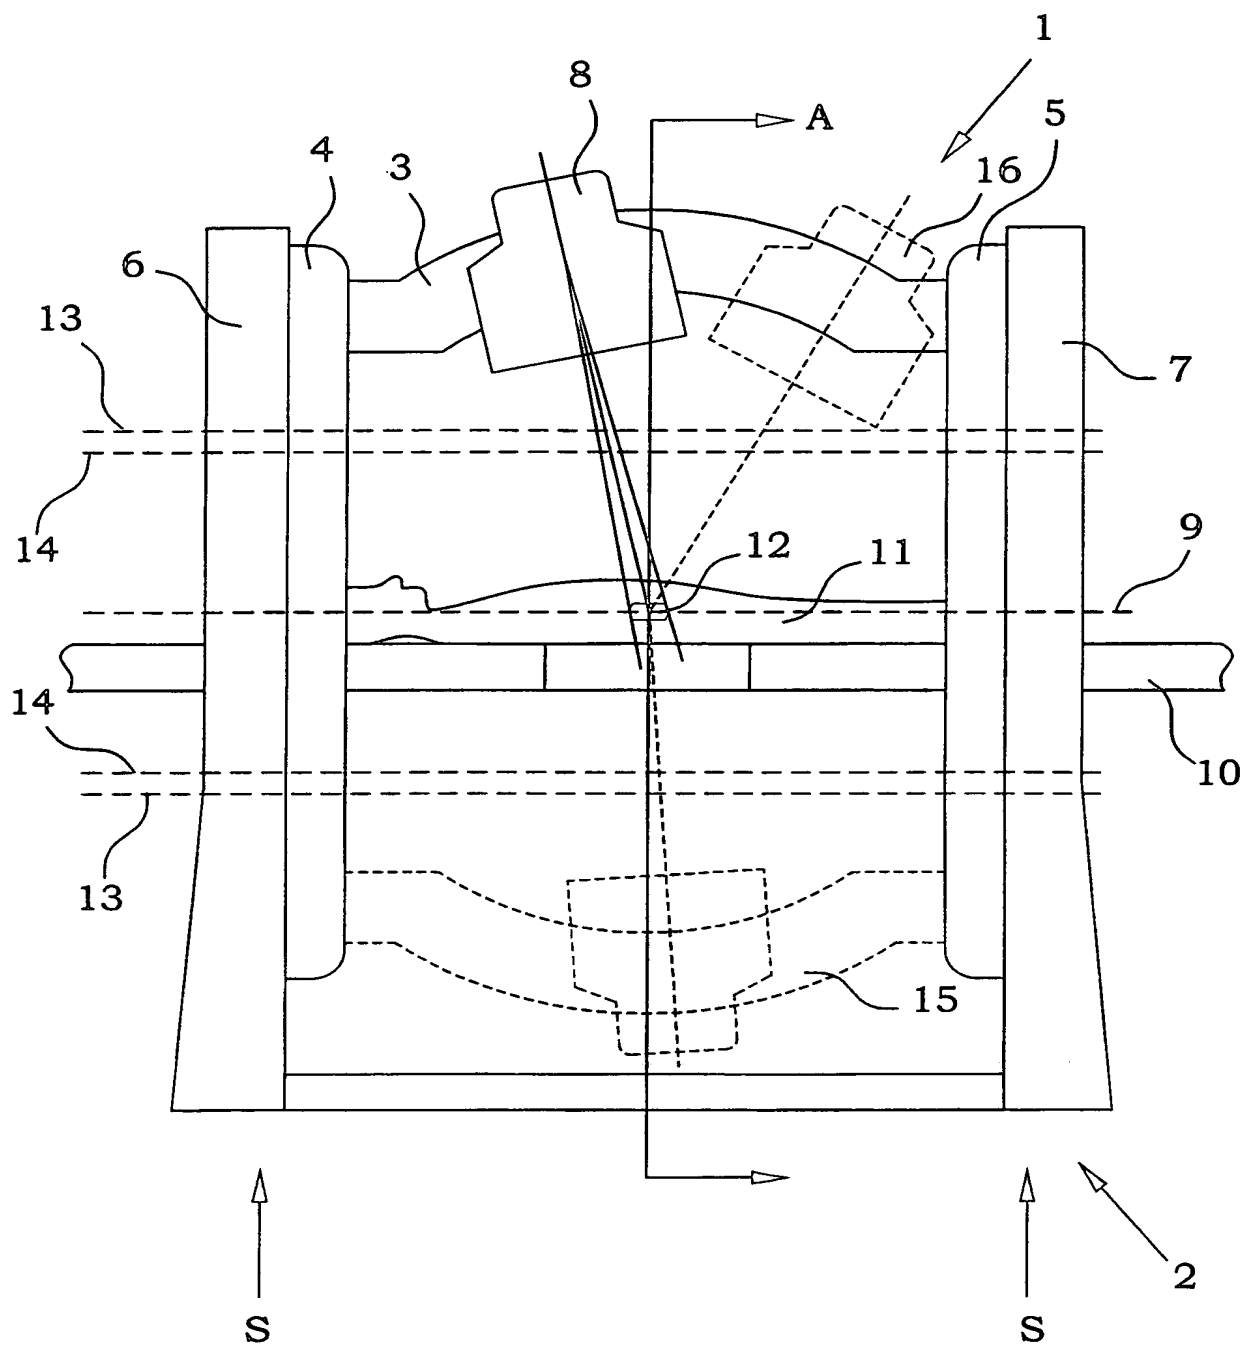


Fig. 1

2/10

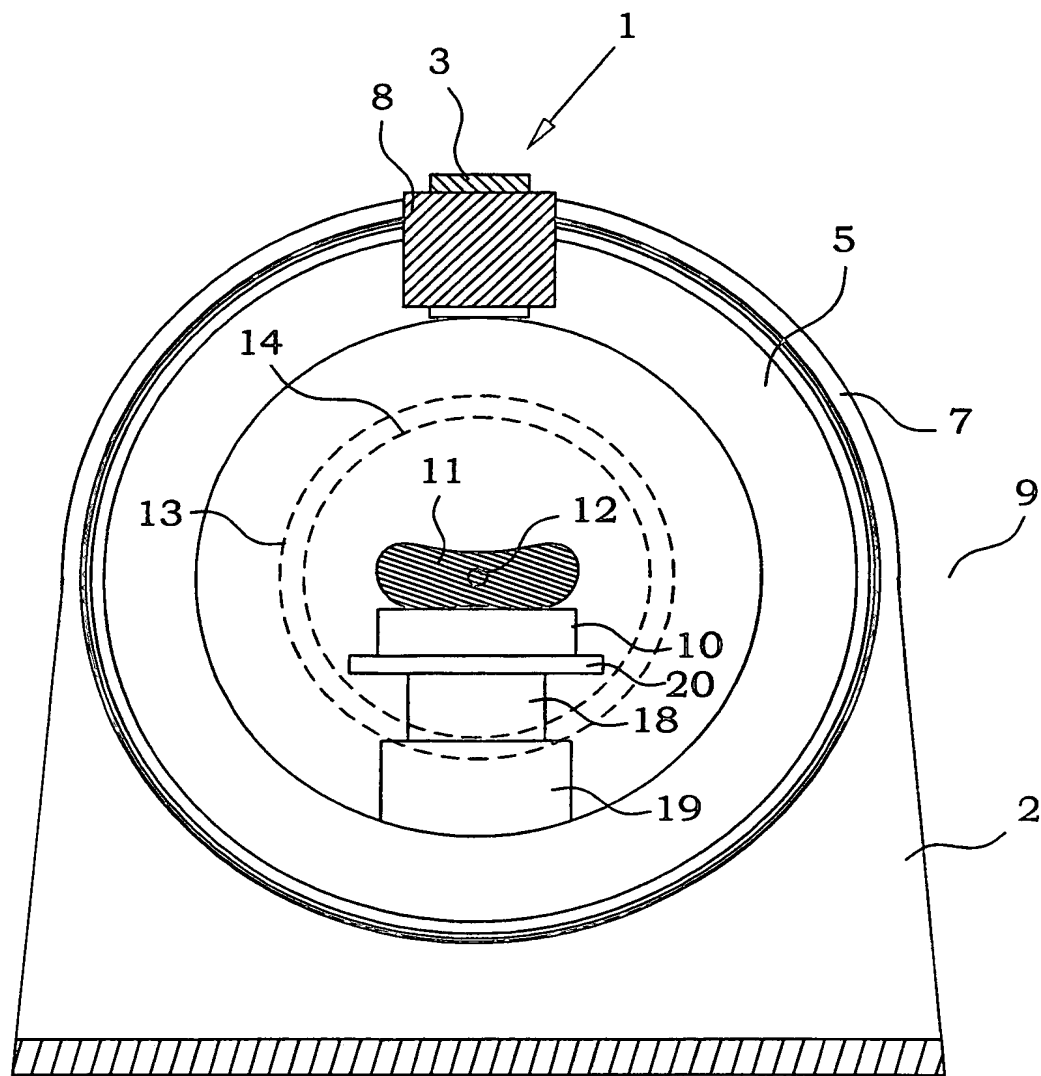


Fig. 2

3/10

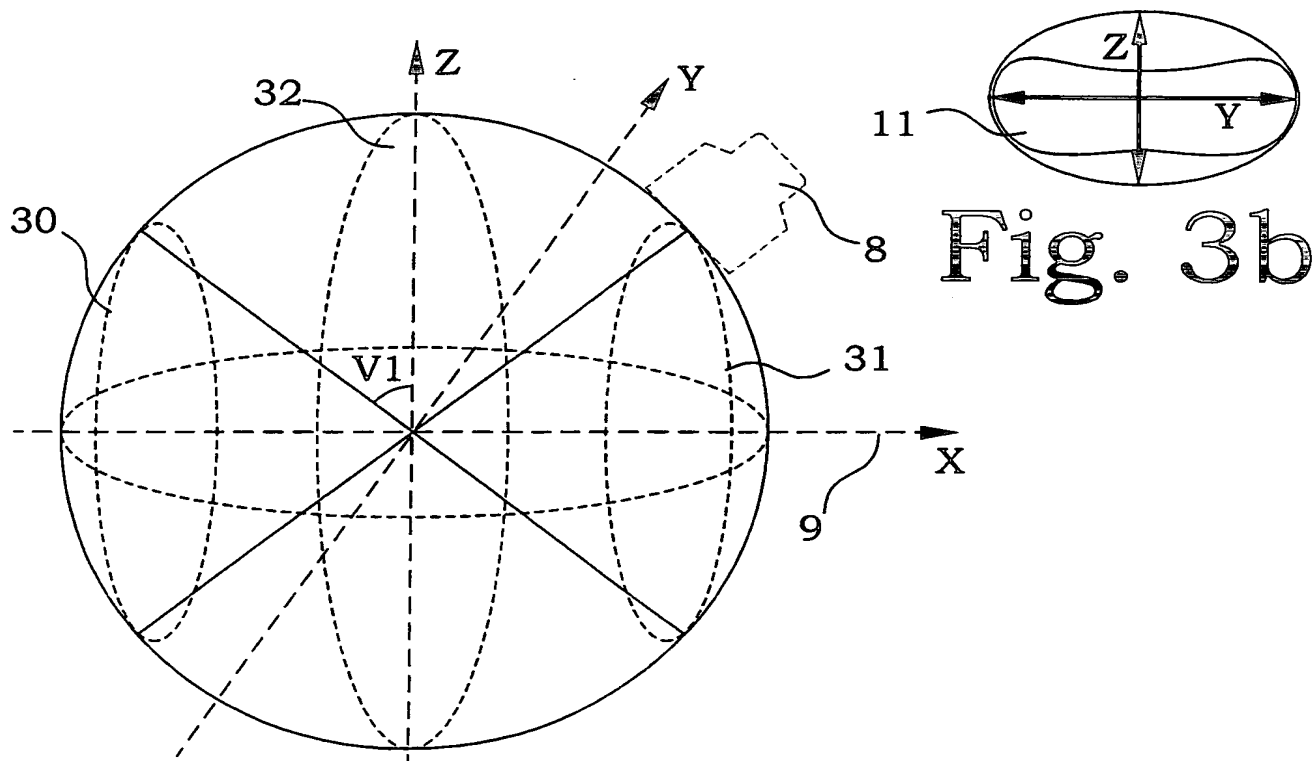
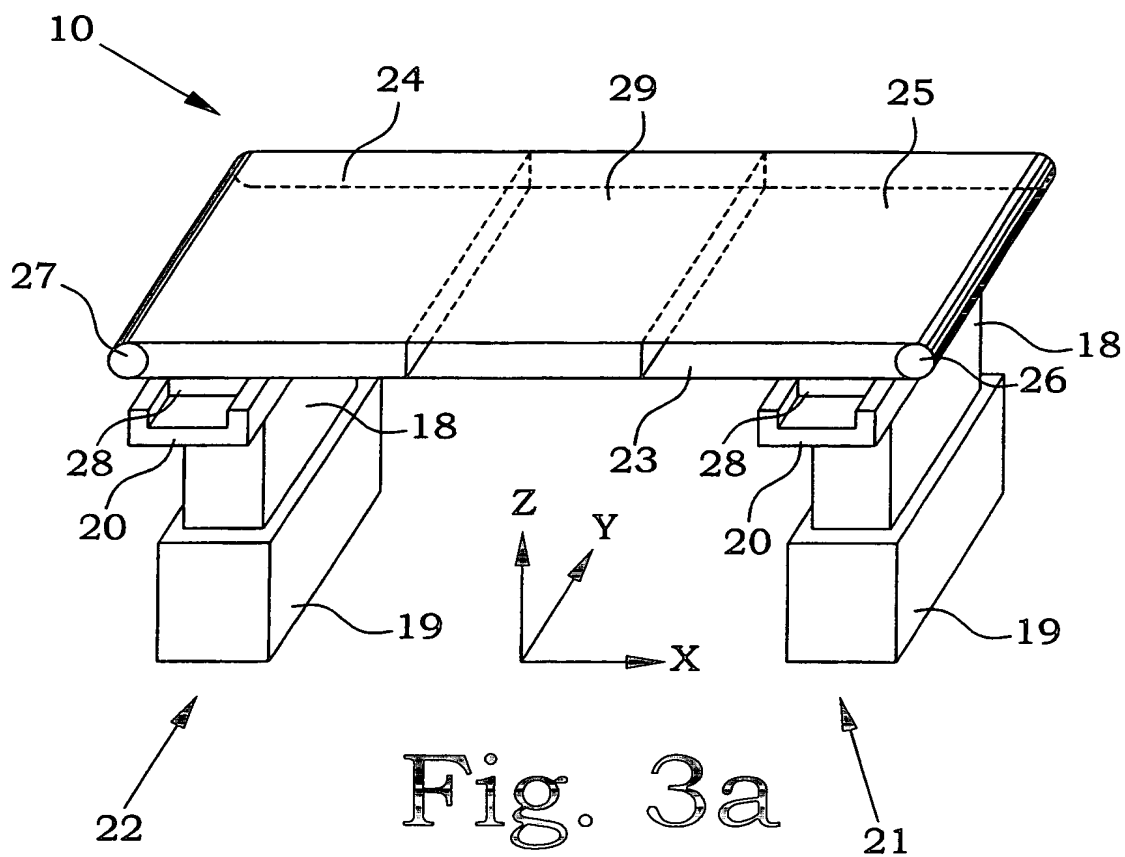


Fig 4

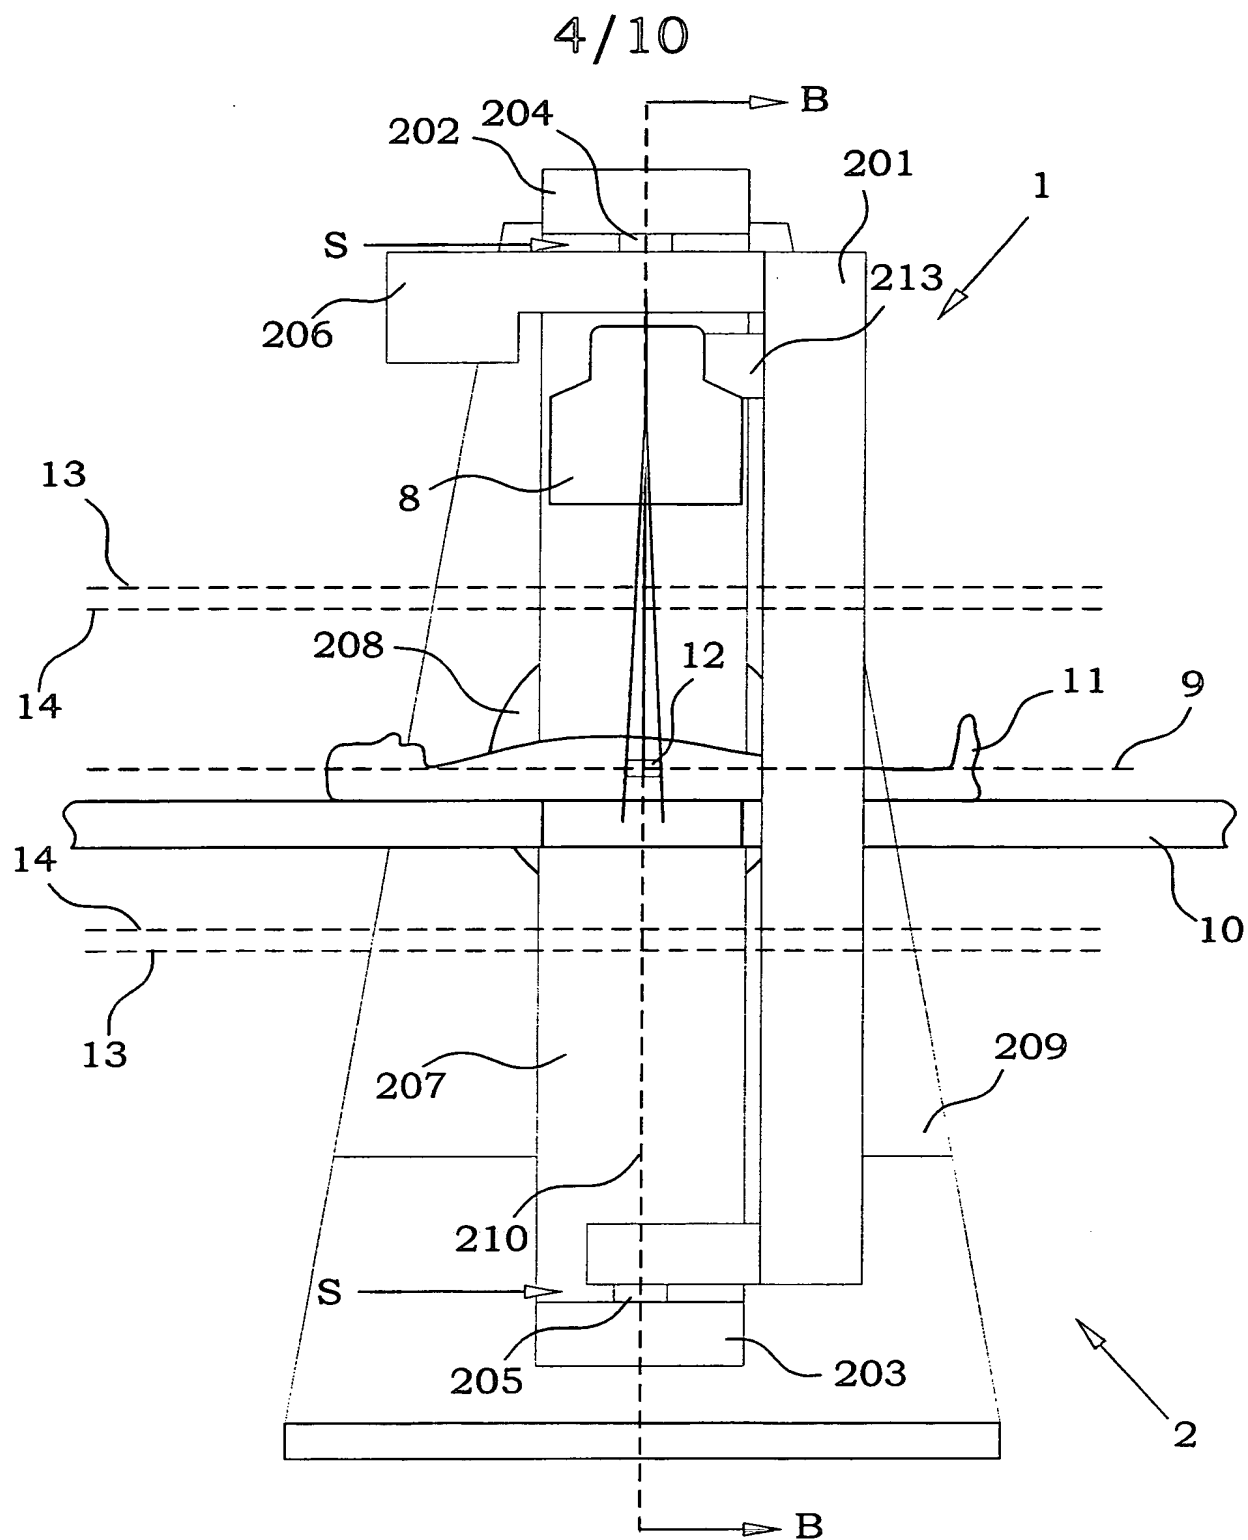


Fig. 5

5/10

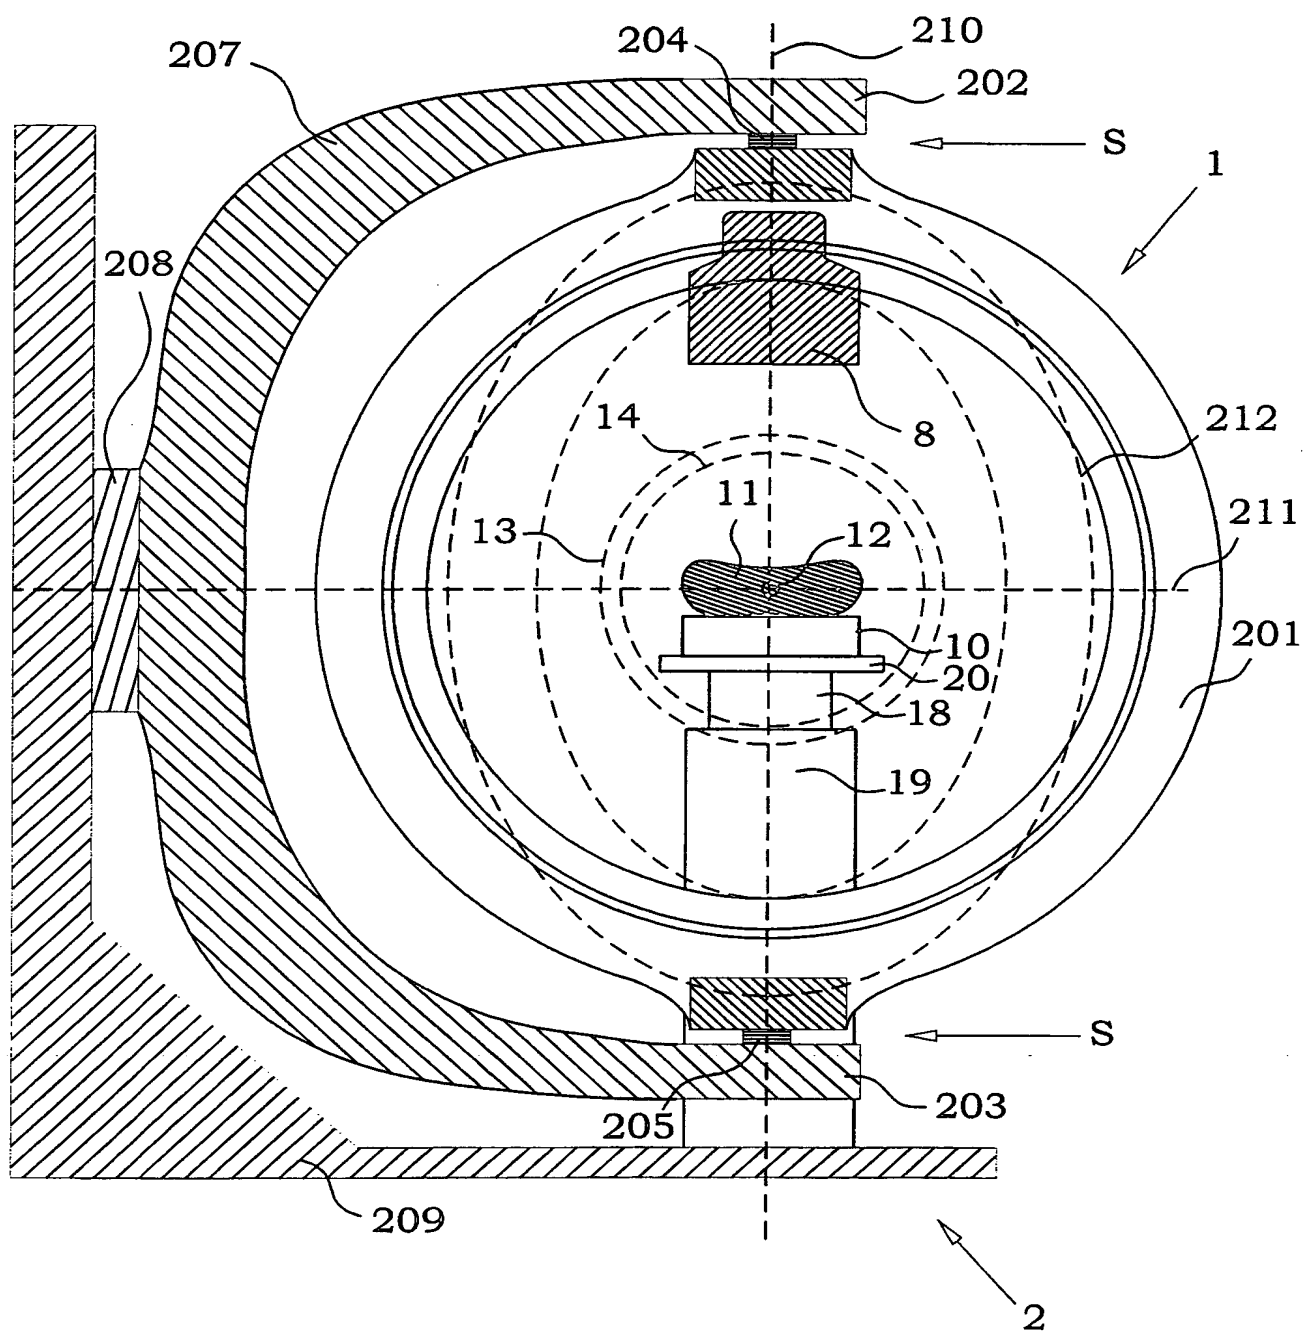


Fig. 6

6/10

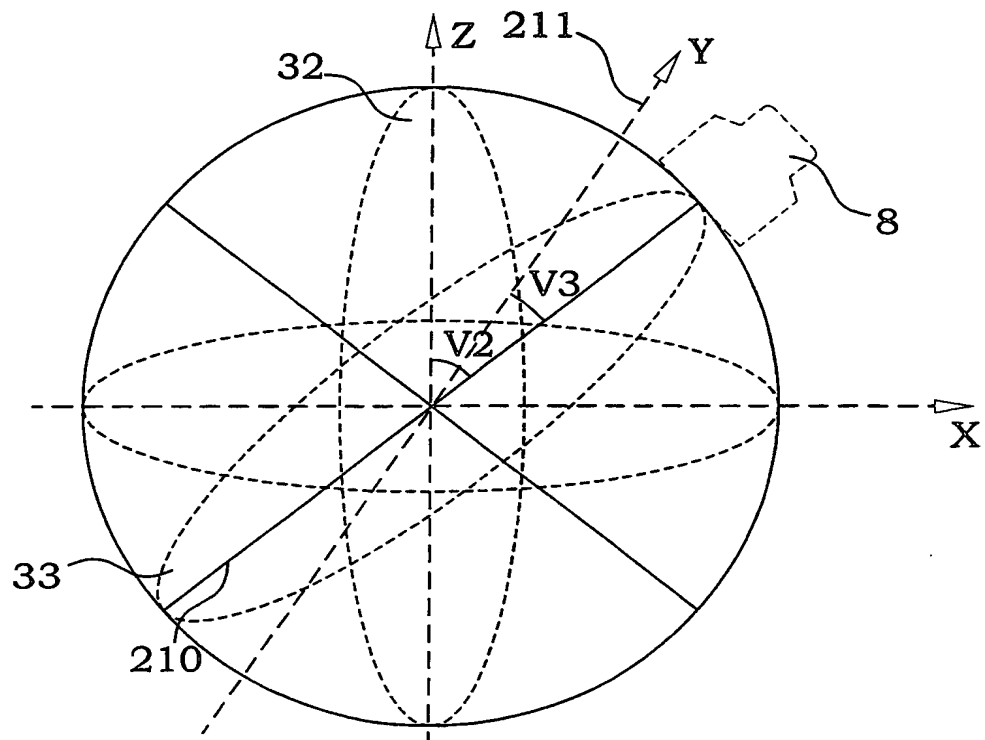


Fig. 7

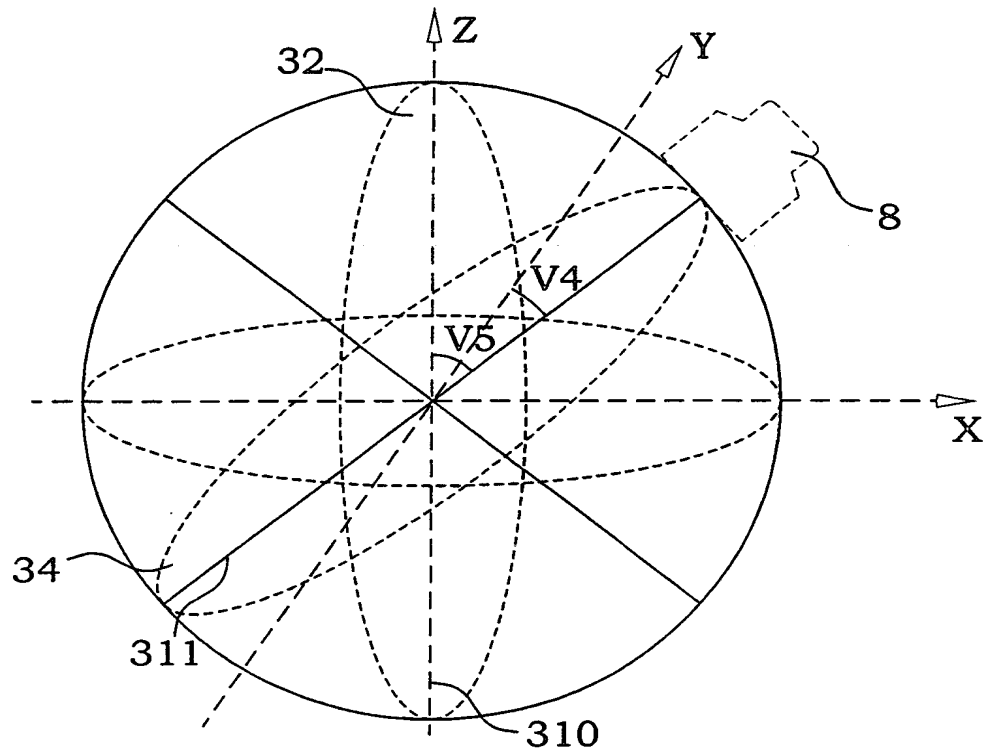


Fig. 10







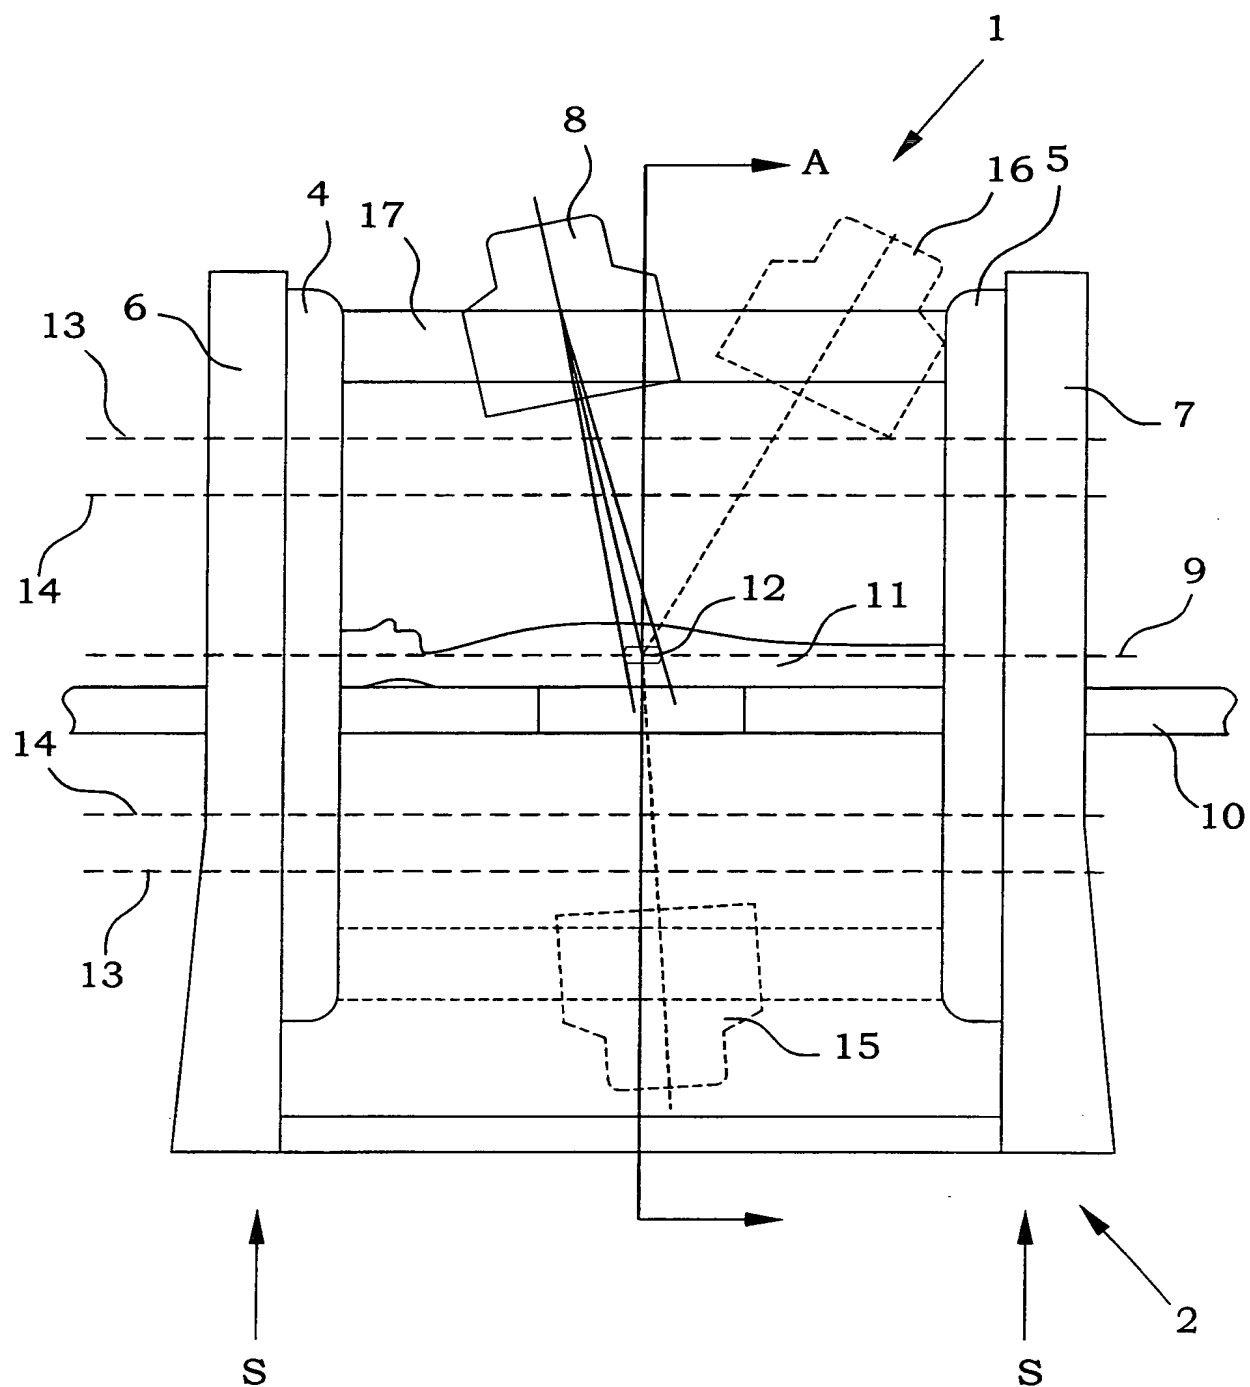


Fig 11

10/10

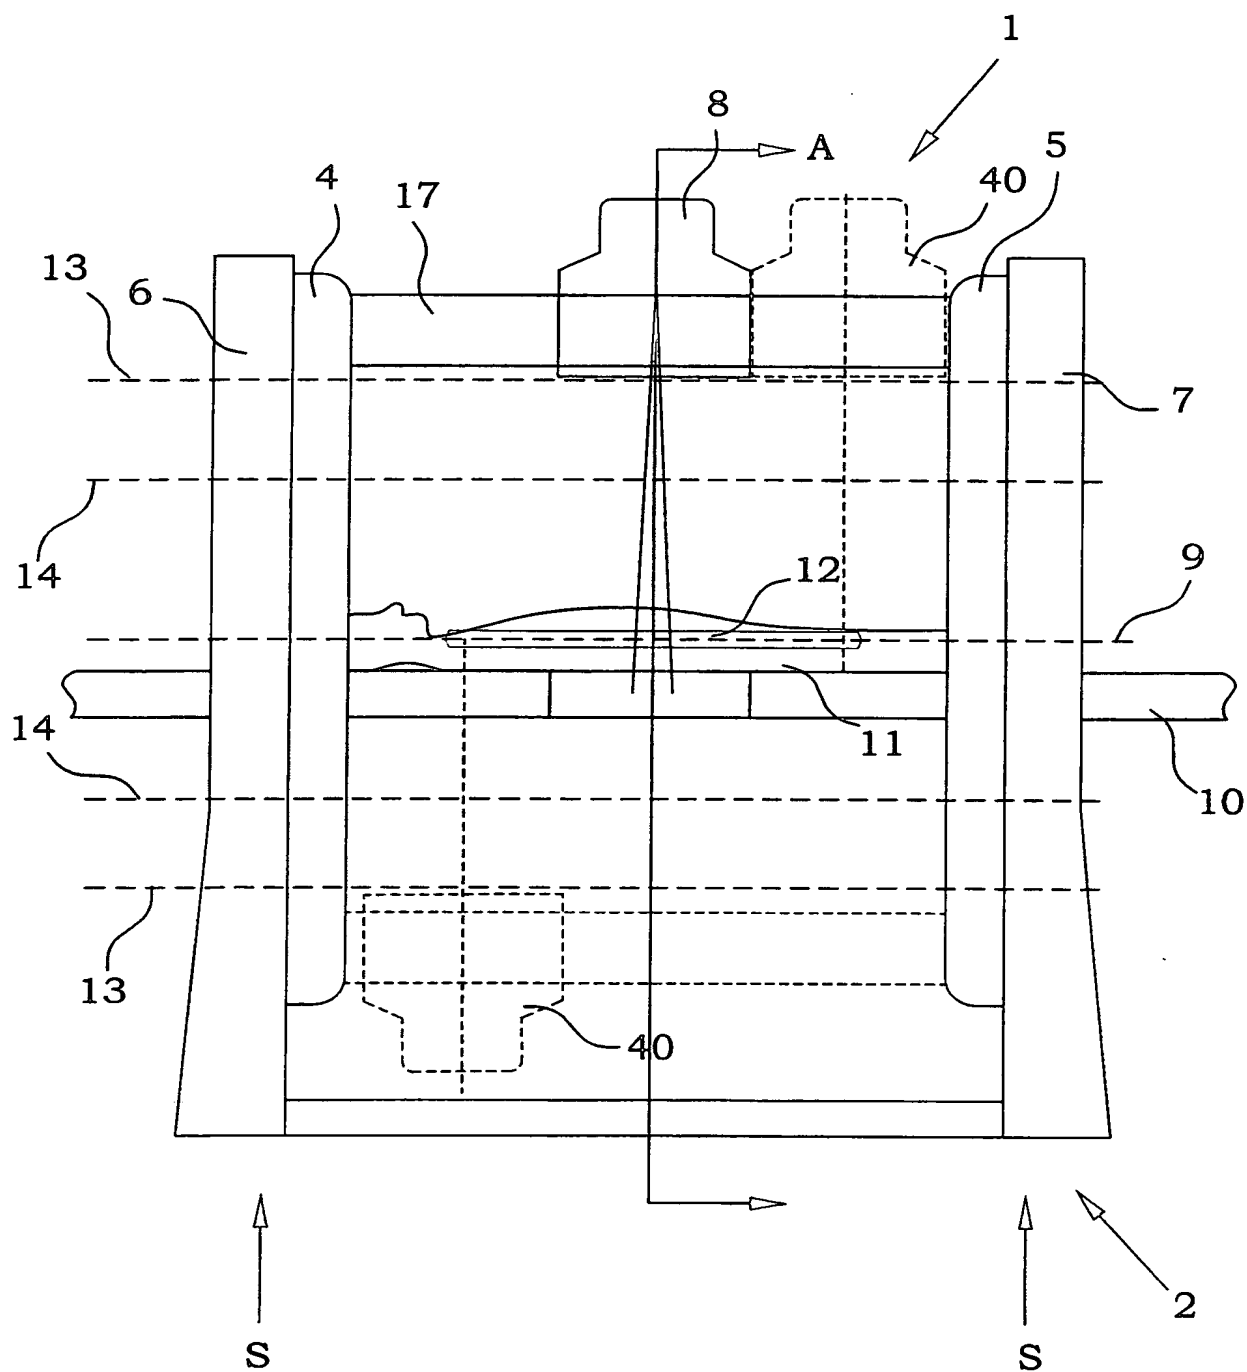


Fig. 12

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/01109

## A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61N 5/01, A61B 6/04

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61N, A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4741015 A (PIERRE CHARRIER), 26 April 1988 (26.04.88), column 1, line 6 - line 60; column 2, line 40 - column 3, line 4, figures; abstract --	1-20
A	WO 8908269 A1 (ANALOGIC CORPORATION), 8 Sept 1989 (08.09.89), figures; claims; abstract --	1-20
A	US 5751781 A (KEVIN J. BROWN ET AL), 12 May 1998 (12.05.98), figures; claims; abstract --	1-20

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

4 October 2000

Date of mailing of the international search report

10 -10- 2000

Name and mailing address of the ISA/  
Swedish Patent Office  
Box 5055, S-102 42 STOCKHOLM  
Facsimile No. +46 8 666 02 86

Authorized officer

Monika Bohlin/MP  
Telephone No. +46 8 782 25 00

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/01109

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	FR 2529088 A1 (MECANIQUE ET CONCEPTIONS INDUSTRIELLES MODERNES (MCIM)), 30 December 1983 (30.12.83), page 2, line 21 - page 4, column 16, figures; claims  --	1-20
A	GB 1129653 A (ARTASHES ERVANDOVICH ATOVMIAN ET AL), 9 October 1968 (09.10.68), page 1, line 24 - line 82; page 3, line 24 - line 58, figures; claims  -- -----	1-20

# INTERNATIONAL SEARCH REPORT

Information on patent family members

01/08/00

International application No.

PCT/SE 00/01109

Patent document cited in search report			Publication date	Patent family member(s)	Publication date
US	4741015	A	26/04/88	NONE	
WO	8908269	A1	08/09/89	DE 3855460 D,T	02/01/97
				DE 3856008 D,T	15/01/98
				DE 3856009 D,T	15/01/98
				DE 3856010 D,T	08/01/98
				DE 3887333 D,T	19/05/94
				EP 0357732 A,B	14/03/90
				EP 0579032 A,B	19/01/94
				EP 0579033 A,B	19/01/94
				EP 0579034 A,B	19/01/94
				EP 0579035 A,B	19/01/94
				JP 2503282 T	11/10/90
				JP 2847655 B	20/01/99
				US RE34379 E	14/09/93
				US RE36099 E	16/02/99
				US 4928283 A	22/05/90
US	5751781	A	12/05/98	GB 2305975 A	23/04/97
				GB 9520567 D	00/00/00
				EP 0814869 A	07/01/98
				JP 10511595 T	10/11/98
				WO 9713552 A	17/04/97
FR	2529088	A1	30/12/83	NONE	
GB	1129653	A	09/10/68	DE 1516402 B	15/01/70
				FR 1454127 A	22/12/66

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
14 December 2000 (14.12.2000)


PCT

(10) International Publication Number  
WO 00/74779 A1

- (51) International Patent Classification<sup>7</sup>: A61N 5/01, A61B 6/04
- (21) International Application Number: PCT/SE00/01109
- (22) International Filing Date: 30 May 2000 (30.05.2000)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data: 9902163-6 9 June 1999 (09.06.1999) SE
- (71) Applicant (for all designated States except US): SCANDITRONIX MEDICAL AB [SE/SE]; Stålgatan 14, S-754 50 Uppsala (SE).
- (72) Inventor; and
- (75) Inventor/Applicant (for US only): NÄFSTADIUS, Peder [SE/SE]; Palissadgränd 66, S-187 66 Täby (SE).
- (74) Agents: HEDBERG, Åke et al.; Aros Patent AB, P.O. Box 1544, S-751 45 Uppsala (SE).
- (81) Designated States (national): AE, AG, AL, AM, AT, AT (utility model), AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, CZ (utility model), DE, DE (utility model), DK, DK (utility model), DM, DZ, EE, EE (utility model), ES, FI, FI (utility model), GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KR (utility model), KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: STABLE ROTATABLE RADIATION GANTRY

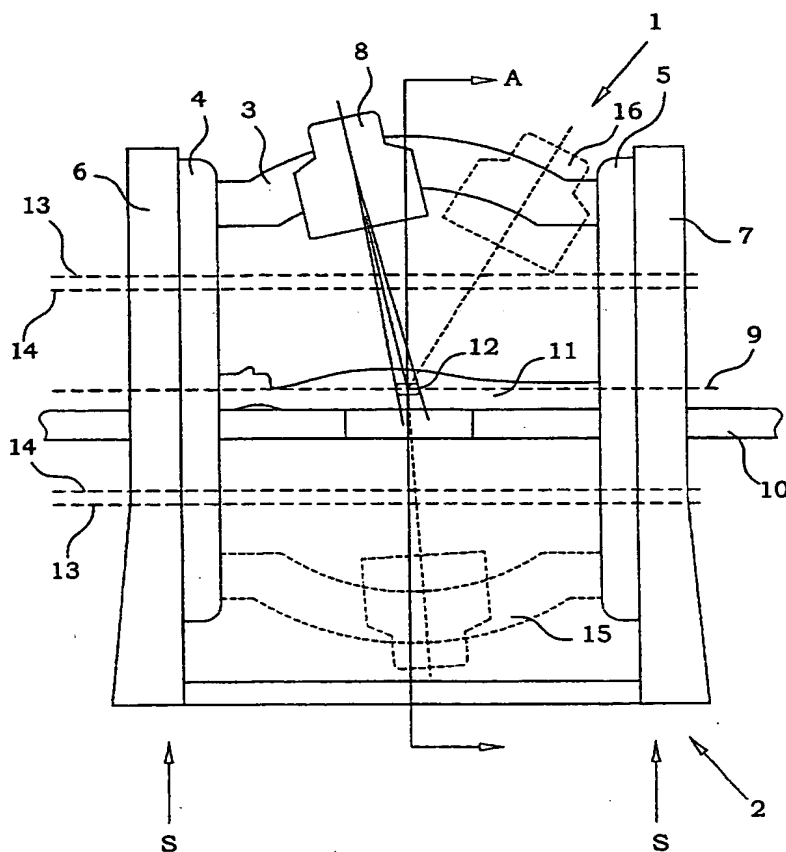

(57) Abstract: The present invention presents an irradiation device providing a free volume around the longitudinal axis of the body (13) around the body to be irradiated. The supporting parts of a gantry (1, 2) are situated substantially radially with respect to the longitudinal axis. The gantry comprises an inner gantry part (1) with at least two supporting locations (S) to an outer gantry portion (2). The support locations (S) are situated at each side of a treatment volume (12). A radiation head (8), mechanically attached to the inner gantry part (1) and arranged to direct radiation to the treatment volume (12) is movable around the treatment volume (12). In preferred embodiments, the parts (20, 21, 22, 23) of the gantry are formed as rings, leaving a free space along the rotational axis (9). A body-supporting couch (10) is arranged along the rotational axis extending through the hollow parts (20, 21, 22, 23). The radiation head (8) is preferably movable in a path also perpendicular to the rotation axis (9). Non-coplanar treatments are thereby possible to obtain. The arrangements are suitable for applying numerical control of the gantry movements. The invention also discloses irradiation methods suitable for such devices.

WO 00/74779 A1

**Published:**

- With international search report.
- Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/01109

## A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61N 5/01, A61B 6/04

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61N, A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4741015 A (PIERRE CHARRIER), 26 April 1988 (26.04.88), column 1, line 6 - line 60; column 2, line 40 - column 3, line 4, figures; abstract --	1-20
A	WO 8908269 A1 (ANALOGIC CORPORATION), 8 Sept 1989 (08.09.89), figures; claims; abstract --	1-20
A	US 5751781 A (KEVIN J. BROWN ET AL), 12 May 1998 (12.05.98), figures; claims; abstract --	1-20

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

4 October 2000

Date of mailing of the international search report

10 -10- 2000

Name and mailing address of the ISA/  
Swedish Patent Office  
Box 5055, S-102 42 STOCKHOLM  
Facsimile No. +46 8 666 02 86

Authorized officer

Monika Bohlin/MP  
Telephone No. +46 8 782 25 00



## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/01109

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	FR 2529088 A1 (MECANIQUE ET CONCEPTIONS INDUSTRIELLES MODERNES (MCIM)), 30 December 1983 (30.12.83), page 2, line 21 - page 4, column 16, figures; claims --	1-20
A	GB 1129653 A (ARTASHES ERVANDOVICH ATOVMIAN ET AL), 9 October 1968 (09.10.68), page 1, line 24 - line 82; page 3, line 24 - line 58, figures; claims -- -----	1-20

**INTERNATIONAL SEARCH REPORT**  
Information on patent family members

01/08/00

International application No.  
PCT/SE 00/01109

Patent document cited in search report			Publication date	Patent family member(s)		Publication date
US	4741015	A	26/04/88	NONE		
WO	8908269	A1	08/09/89	DE	3855460 D,T	02/01/97
				DE	3856008 D,T	15/01/98
				DE	3856009 D,T	15/01/98
				DE	3856010 D,T	08/01/98
				DE	3887333 D,T	19/05/94
				EP	0357732 A,B	14/03/90
				EP	0579032 A,B	19/01/94
				EP	0579033 A,B	19/01/94
				EP	0579034 A,B	19/01/94
				EP	0579035 A,B	19/01/94
				JP	2503282 T	11/10/90
				JP	2847655 B	20/01/99
				US	RE34379 E	14/09/93
				US	RE36099 E	16/02/99
				US	4928283 A	22/05/90
US	5751781	A	12/05/98	GB	2305975 A	23/04/97
				GB	9520567 D	00/00/00
				EP	0814869 A	07/01/98
				JP	10511595 T	10/11/98
				WO	9713552 A	17/04/97
FR	2529088	A1	30/12/83	NONE		
GB	1129653	A	09/10/68	DE	1516402 B	15/01/70
				FR	1454127 A	22/12/66